

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
 Data File : BN029933.D
 Acq On : 22 Feb 2024 18:39
 Operator : MA/JU
 Sample : PB159102BL
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK102

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029933.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.317	35	39	46	rBV	70720	92044	2.22%	0.189%
2	3.723	105	108	127	rBV	770367	1271287	30.60%	2.609%
3	4.040	158	162	169	rVB3	34565	62386	1.50%	0.128%
4	4.223	189	193	195	rBV4	6425	8273	0.20%	0.017%
5	4.276	198	202	208	rVB3	23339	32904	0.79%	0.068%
6	4.423	224	227	231	rVB3	10481	15296	0.37%	0.031%
7	4.605	254	258	264	rVB	48583	68505	1.65%	0.141%
8	4.664	264	268	278	rVB2	16588	38529	0.93%	0.079%
9	5.758	451	454	461	rVB8	6257	10668	0.26%	0.022%
10	6.187	521	527	531	rVB9	4659	9861	0.24%	0.020%
11	6.693	608	613	614	rBV5	3465	4273	0.10%	0.009%
12	7.022	662	669	686	rBV	981213	1604866	38.63%	3.294%
13	7.199	693	699	716	rVB	776665	1249602	30.08%	2.565%
14	7.387	724	731	742	rBV	986210	1589024	38.25%	3.261%
15	7.564	757	761	769	rVB7	5992	13194	0.32%	0.027%
16	7.858	803	811	820	rBV	739925	1176546	28.32%	2.415%
17	8.016	837	838	844	rVB4	3612	4354	0.10%	0.009%
18	8.099	847	852	856	rBV5	7275	11756	0.28%	0.024%
19	8.569	925	932	944	rBV	1128830	1863550	44.85%	3.825%
20	8.840	974	978	982	rVB6	3193	4488	0.11%	0.009%
21	8.881	982	985	989	rBV6	3250	5013	0.12%	0.010%
22	9.022	1002	1009	1020	rBV	913549	1504890	36.22%	3.089%
23	9.740	1124	1131	1144	rBV	716159	1206861	29.05%	2.477%
24	10.275	1214	1222	1239	rBV	1069459	1820560	43.82%	3.737%
25	10.516	1260	1263	1271	rVB8	3366	6491	0.16%	0.013%
26	10.652	1279	1286	1296	rVB	954639	1628907	39.21%	3.343%
27	10.799	1303	1311	1331	rBV	1011255	1892073	45.54%	3.883%
28	11.416	1411	1416	1419	rBV7	4395	6680	0.16%	0.014%
29	11.493	1423	1429	1431	rBV6	3192	4843	0.12%	0.010%
30	12.246	1551	1557	1564	rBV2	16497	28757	0.69%	0.059%
31	13.404	1749	1754	1762	rBV4	15410	24634	0.59%	0.051%
32	13.922	1835	1842	1853	rBV	1720589	2399162	57.75%	4.924%
33	14.193	1881	1888	1898	rBV	1987018	2899386	69.79%	5.951%
34	14.498	1933	1940	1954	rBV	1317587	1914221	46.07%	3.929%
35	14.710	1968	1976	2001	rBV	531038	1116468	26.87%	2.291%
36	15.498	2103	2110	2122	rBV	2386581	3498188	84.20%	7.180%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
 Data File : BN029933.D
 Acq On : 22 Feb 2024 18:39
 Operator : MA/JU
 Sample : PB159102BL
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK102

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

37	15.622	2125	2131	2142	rVV	650837	926658	22.30%	1.902%
38	15.734	2145	2150	2155	rVB3	11843	20980	0.50%	0.043%
39	16.287	2240	2244	2247	rBV5	6295	9179	0.22%	0.019%
40	16.934	2351	2354	2360	rVB7	2740	4345	0.10%	0.009%
41	17.034	2367	2371	2376	rBV5	3938	5812	0.14%	0.012%
42	17.251	2402	2408	2418	rBV	1559384	2200877	52.97%	4.517%
43	17.351	2418	2425	2441	rVB2	2617429	3708066	89.25%	7.611%
44	18.504	2616	2621	2625	rBV8	3591	7886	0.19%	0.016%
45	19.216	2738	2742	2748	rVB4	28066	42234	1.02%	0.087%
46	19.286	2750	2754	2761	rVV	23711	37452	0.90%	0.077%
47	19.369	2764	2768	2772	rVV6	4928	6628	0.16%	0.014%
48	19.610	2806	2809	2810	rBV3	8346	9191	0.22%	0.019%
49	19.651	2810	2816	2826	rVV	2948928	4154665	100.00%	8.527%
50	21.457	3117	3123	3136	rBV	1654810	2226023	53.58%	4.569%
51	23.669	3491	3499	3512	rBV2	1983583	3998297	96.24%	8.206%
52	23.822	3518	3525	3542	rVB	1085515	2275610	54.77%	4.671%




Sum of corrected areas: 48722443

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029933.D
Acq On : 22 Feb 2024 18:39
Operator : MA/JU
Sample : PB159102BL
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK102

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

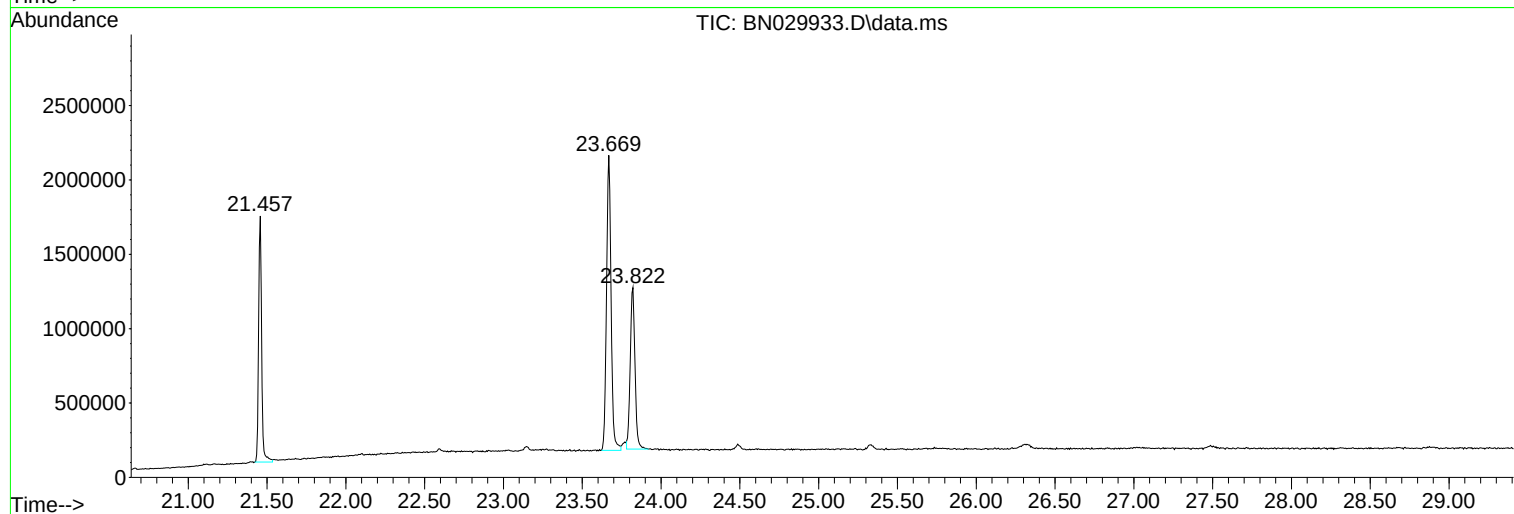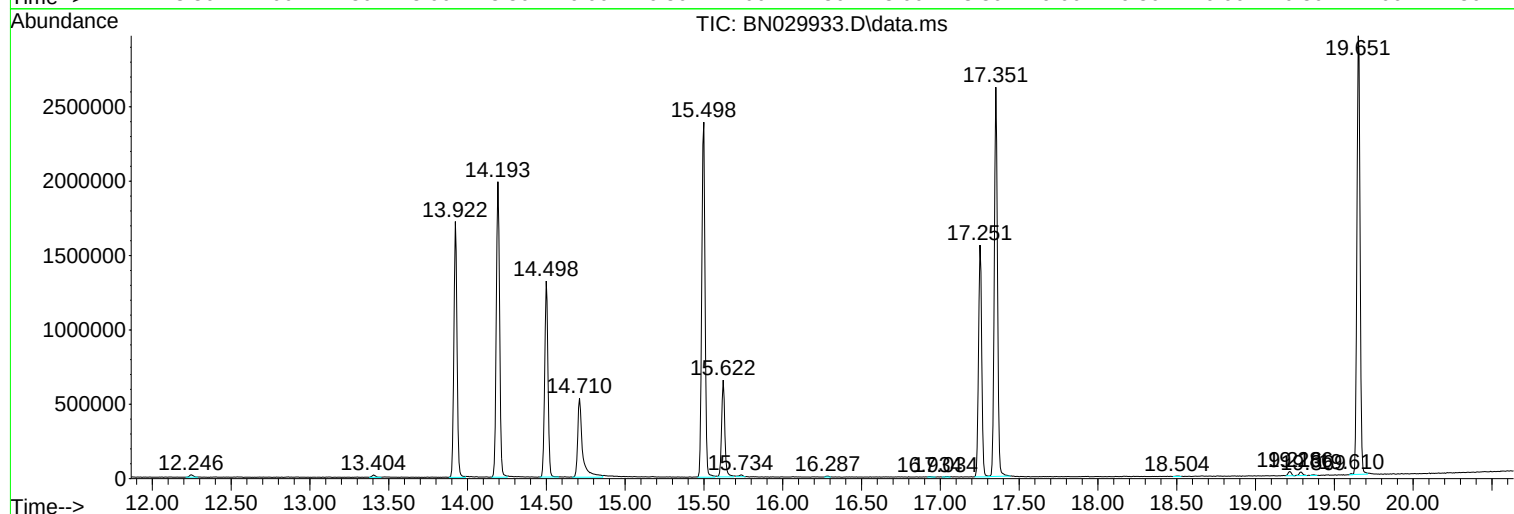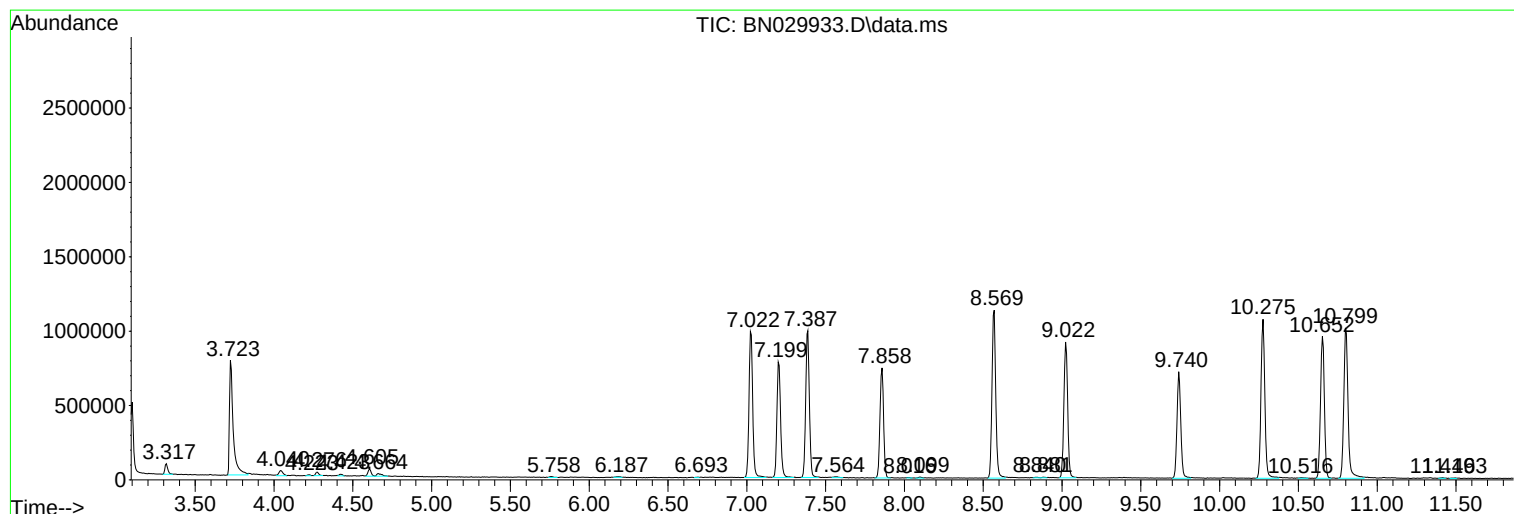

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029933.D
Acq On : 22 Feb 2024 18:39
Operator : MA/JU
Sample : PB159102BL
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK102

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029933.D
Acq On : 22 Feb 2024 18:39
Operator : MA/JU
Sample : PB159102BL
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK102

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------