

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
 Data File : BN029934.D
 Acq On : 22 Feb 2024 19:14
 Operator : MA/JU
 Sample : PB159100BL
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK100

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029934.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.317	35	39	45	rVB	71982	89359	2.06%	0.180%
2	3.723	105	108	132	rBV	810771	1332903	30.71%	2.682%
3	4.046	158	163	168	rBV4	31526	54830	1.26%	0.110%
4	4.222	189	193	197	rBV5	6796	9530	0.22%	0.019%
5	4.275	198	202	208	rVV2	27474	37287	0.86%	0.075%
6	4.428	224	228	232	rVB3	11852	16373	0.38%	0.033%
7	4.552	247	249	253	rBV5	5691	7381	0.17%	0.015%
8	4.605	254	258	263	rVB	50082	67993	1.57%	0.137%
9	4.658	264	267	269	rBV2	15019	19778	0.46%	0.040%
10	5.758	445	454	458	rBV8	7043	14392	0.33%	0.029%
11	6.187	522	527	532	rBV9	5031	9618	0.22%	0.019%
12	6.652	603	606	608	rBV4	3814	5976	0.14%	0.012%
13	7.022	662	669	678	rBV	1027821	1676790	38.63%	3.374%
14	7.205	693	700	713	rVB	802086	1304789	30.06%	2.626%
15	7.387	723	731	747	rBV	1047736	1683618	38.79%	3.388%
16	7.563	757	761	765	rBV7	5458	7487	0.17%	0.015%
17	7.669	776	779	787	rBV8	2653	5863	0.14%	0.012%
18	7.858	803	811	820	rBV	712260	1112406	25.63%	2.239%
19	8.016	834	838	844	rVB6	3200	5243	0.12%	0.011%
20	8.099	848	852	856	rVB5	5533	8675	0.20%	0.017%
21	8.569	925	932	943	rBV	1199117	1945745	44.83%	3.915%
22	8.887	984	986	993	rVB8	3688	5877	0.14%	0.012%
23	9.022	1000	1009	1019	rBV	949655	1568771	36.14%	3.157%
24	9.310	1053	1058	1059	rBV4	2645	4367	0.10%	0.009%
25	9.740	1124	1131	1146	rVV	755834	1252069	28.85%	2.520%
26	10.010	1173	1177	1181	rBV5	3861	7855	0.18%	0.016%
27	10.275	1213	1222	1240	rBV	1109584	1906266	43.92%	3.836%
28	10.410	1243	1245	1249	rVB5	3215	4343	0.10%	0.009%
29	10.522	1258	1264	1269	rVB9	4022	7393	0.17%	0.015%
30	10.652	1278	1286	1297	rVB	919540	1548410	35.68%	3.116%
31	10.799	1303	1311	1332	rBV	1056854	1958981	45.14%	3.942%
32	11.040	1347	1352	1354	rBV5	4471	5688	0.13%	0.011%
33	11.299	1392	1396	1400	rBV6	3590	6528	0.15%	0.013%
34	11.416	1410	1416	1420	rVB9	3970	6698	0.15%	0.013%
35	12.246	1551	1557	1563	rBV2	15670	29722	0.68%	0.060%
36	13.404	1748	1754	1760	rVB4	13200	21296	0.49%	0.043%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
 Data File : BN029934.D
 Acq On : 22 Feb 2024 19:14
 Operator : MA/JU
 Sample : PB159100BL
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK100

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

37	13.475	1763	1766	1771	rVB5	2822	4536	0.10%	0.009%
38	13.922	1835	1842	1855	rBV	1781935	2485803	57.27%	5.002%
39	14.193	1881	1888	1899	rBV	2061492	3037085	69.98%	6.112%
40	14.498	1933	1940	1950	rBV	1233581	1796074	41.38%	3.614%
41	14.710	1969	1976	2006	rBV	581813	1188968	27.39%	2.393%
42	15.498	2102	2110	2124	rBV	2464129	3651170	84.12%	7.347%
43	15.622	2124	2131	2147	rVV	685576	1003494	23.12%	2.019%
44	15.734	2147	2150	2159	rVB4	16052	25398	0.59%	0.051%
45	16.063	2200	2206	2212	rBV8	3718	6402	0.15%	0.013%
46	16.287	2239	2244	2249	rVB5	8015	10902	0.25%	0.022%
47	17.039	2369	2372	2377	rBV6	4047	6028	0.14%	0.012%
48	17.251	2402	2408	2418	rBV	1467889	2086267	48.07%	4.198%
49	17.351	2418	2425	2448	rVB	2765526	3904136	89.95%	7.856%
50	19.216	2737	2742	2747	rVB4	29503	41689	0.96%	0.084%
51	19.286	2749	2754	2762	rVV	25436	39757	0.92%	0.080%
52	19.369	2765	2768	2771	rVB4	4329	4716	0.11%	0.009%
53	19.610	2806	2809	2810	rBV3	7935	7520	0.17%	0.015%
54	19.651	2810	2816	2827	rVV	3113442	4340229	100.00%	8.734%
55	21.457	3117	3123	3134	rBV	1489526	2050693	47.25%	4.127%
56	23.669	3491	3499	3511	rBV2	2013907	4102625	94.53%	8.256%
57	23.816	3518	3524	3539	rVB	1015108	2149900	49.53%	4.326%




Sum of corrected areas: 49693692

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029934.D
Acq On : 22 Feb 2024 19:14
Operator : MA/JU
Sample : PB159100BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK100

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

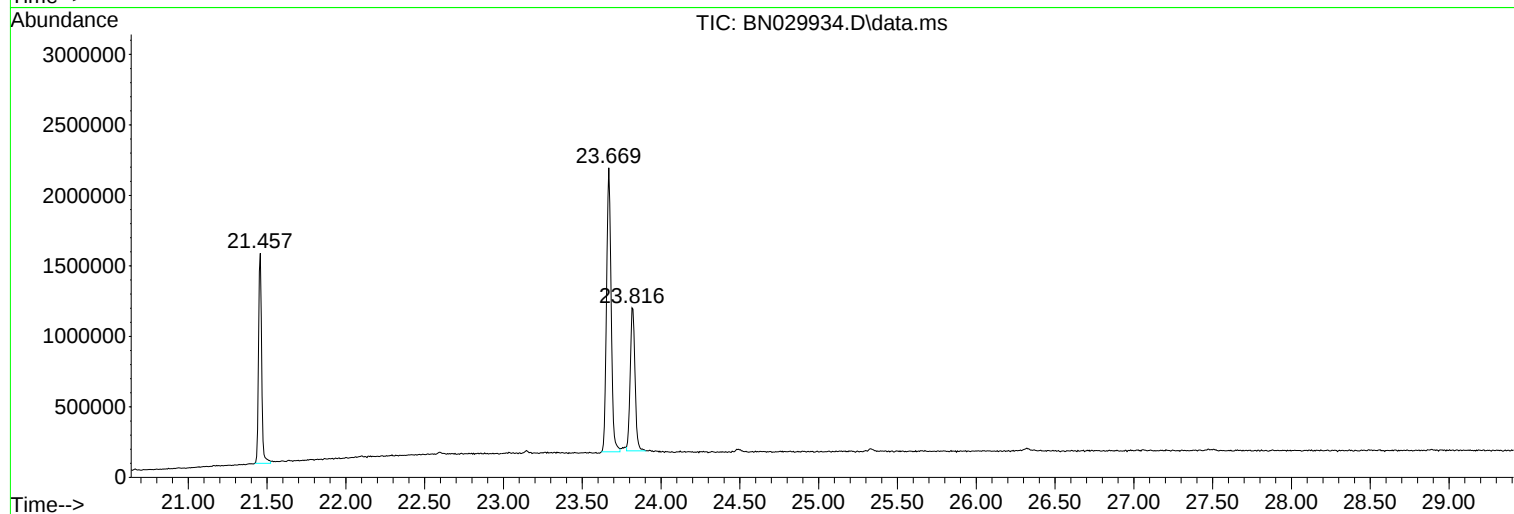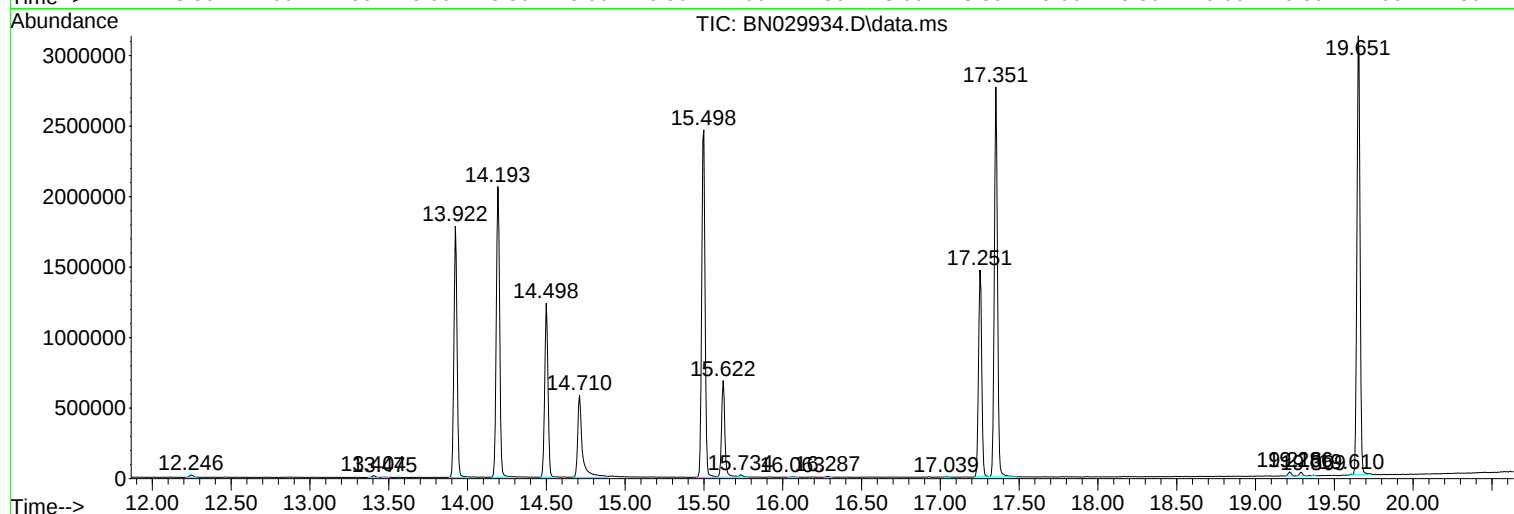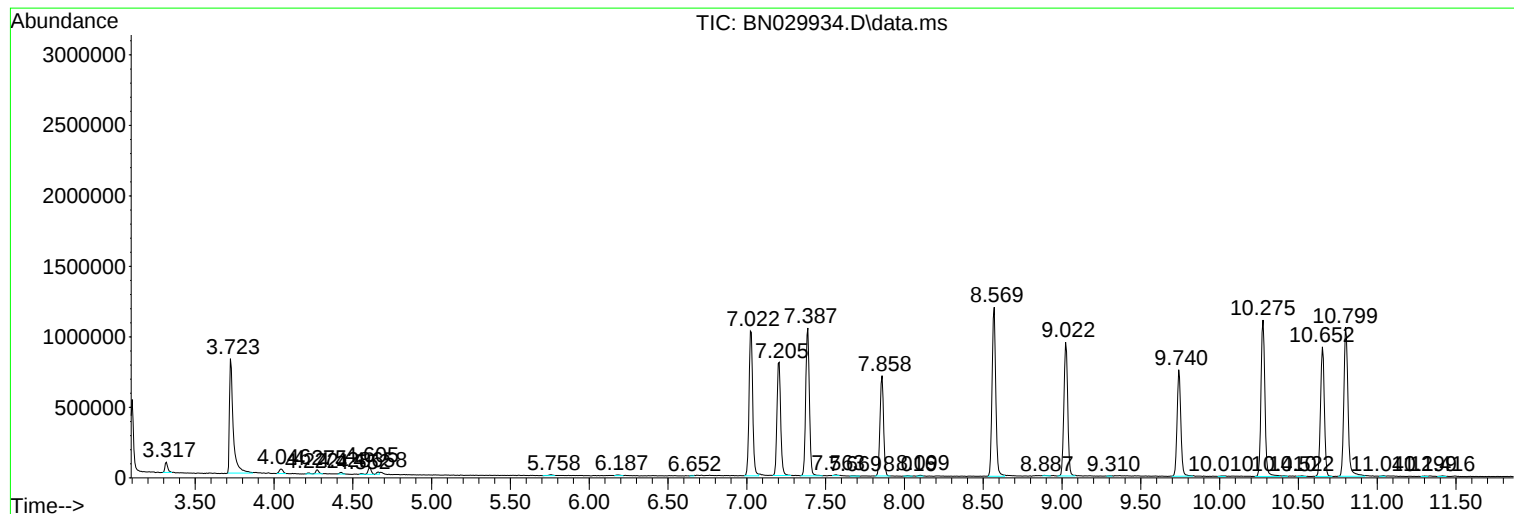

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029934.D
Acq On : 22 Feb 2024 19:14
Operator : MA/JU
Sample : PB159100BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK100

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029934.D
Acq On : 22 Feb 2024 19:14
Operator : MA/JU
Sample : PB159100BL
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK100

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc