

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
 Data File : BN029937.D
 Acq On : 22 Feb 2024 21:03
 Operator : MA/JU
 Sample : P1494-04
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH3Y6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029937.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.281	29	33	36	rBV3	35275	47839	1.03%	0.121%
2	3.316	36	39	45	rVB2	29975	37406	0.81%	0.095%
3	3.734	108	110	126	rBV	128026	270723	5.84%	0.687%
4	4.046	159	163	172	rVB	15203	25696	0.55%	0.065%
5	7.022	663	669	680	rVB	136120	231825	5.00%	0.589%
6	7.199	693	699	710	rBV	596891	970228	20.95%	2.463%
7	7.387	724	731	740	rBV	554169	907770	19.60%	2.305%
8	7.857	804	811	818	rBV	579928	932906	20.14%	2.368%
9	8.569	925	932	944	rBV	381965	646486	13.96%	1.641%
10	9.022	1001	1009	1021	rBV	723258	1197524	25.85%	3.040%
11	9.740	1120	1131	1144	rBV	526342	902705	19.49%	2.292%
12	10.275	1214	1222	1236	rBV	743939	1274323	27.51%	3.235%
13	10.651	1279	1286	1296	rVB	764212	1291975	27.89%	3.280%
14	10.798	1304	1311	1326	rBV	683576	1306514	28.21%	3.317%
15	12.251	1550	1558	1563	rBV2	12609	24540	0.53%	0.062%
16	13.328	1736	1741	1746	rBV6	5805	8207	0.18%	0.021%
17	13.404	1748	1754	1760	rBV2	12553	22077	0.48%	0.056%
18	13.922	1834	1842	1858	rBV	1478092	2075304	44.80%	5.269%
19	14.192	1881	1888	1903	rBV2	1625855	2423417	52.32%	6.153%
20	14.498	1933	1940	1950	rBV	1041295	1520107	32.82%	3.859%
21	14.716	1970	1977	1993	rBV2	50504	146523	3.16%	0.372%
22	14.910	2006	2010	2012	rBV4	3837	4795	0.10%	0.012%
23	15.498	2103	2110	2125	rBV	2091078	3107141	67.08%	7.888%
24	15.622	2125	2131	2144	rVV	695145	1008140	21.77%	2.559%
25	15.739	2146	2151	2156	rVB7	9199	17282	0.37%	0.044%
26	16.280	2240	2243	2248	rVB5	7943	9959	0.22%	0.025%
27	16.928	2349	2353	2359	rBV7	4132	6963	0.15%	0.018%
28	17.251	2402	2408	2419	rBV	1240731	1773122	38.28%	4.502%
29	17.351	2419	2425	2443	rVV2	2892567	4126099	89.08%	10.475%
30	17.492	2447	2449	2453	rVB5	3728	4871	0.11%	0.012%
31	18.163	2558	2563	2570	rBV2	46436	71320	1.54%	0.181%
32	18.233	2573	2575	2581	rVV6	4189	7634	0.16%	0.019%
33	18.427	2604	2608	2612	rVB2	21493	28103	0.61%	0.071%
34	18.492	2616	2619	2622	rVV4	5131	6263	0.14%	0.016%
35	18.604	2634	2638	2641	rBV6	2700	4835	0.10%	0.012%
36	18.645	2643	2645	2649	rBV4	4116	5663	0.12%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
 Data File : BN029937.D
 Acq On : 22 Feb 2024 21:03
 Operator : MA/JU
 Sample : P1494-04
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH3Y6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

37	19.216	2737	2742	2746	rBV3	31826	44548	0.96%	0.113%
38	19.286	2749	2754	2758	rBV	31529	48425	1.05%	0.123%
39	19.333	2758	2762	2765	rVB5	8151	10306	0.22%	0.026%
40	19.451	2778	2782	2785	rBV3	24839	34193	0.74%	0.087%
41	19.604	2805	2808	2810	rBV3	9544	10346	0.22%	0.026%
42	19.651	2810	2816	2825	rVV	3555411	4631870	100.00%	11.759%
43	20.663	2985	2988	2993	rBV6	10116	17246	0.37%	0.044%
44	21.186	3075	3077	3085	rVB5	32900	51329	1.11%	0.130%
45	21.451	3117	3122	3135	rBV	1276937	1809019	39.06%	4.593%
46	23.662	3491	3498	3511	rBV2	2116095	4441978	95.90%	11.277%
47	23.815	3517	3524	3536	rVB	882288	1843546	39.80%	4.680%




Sum of corrected areas: 39389091

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029937.D
Acq On : 22 Feb 2024 21:03
Operator : MA/JU
Sample : P1494-04
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3Y6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

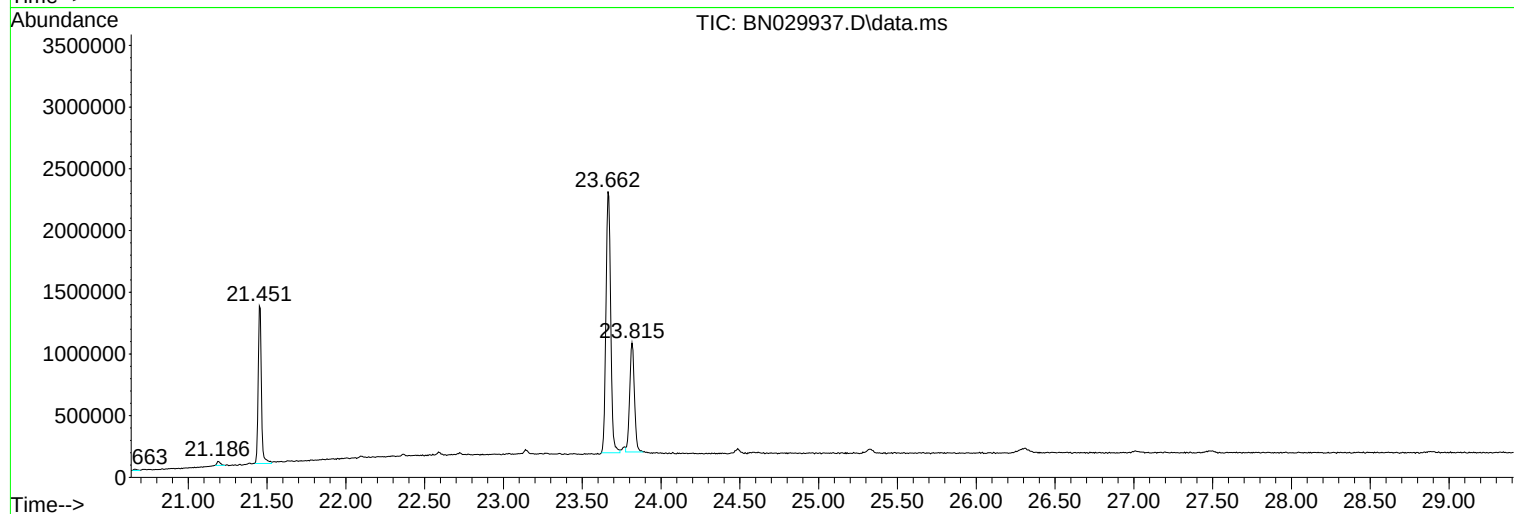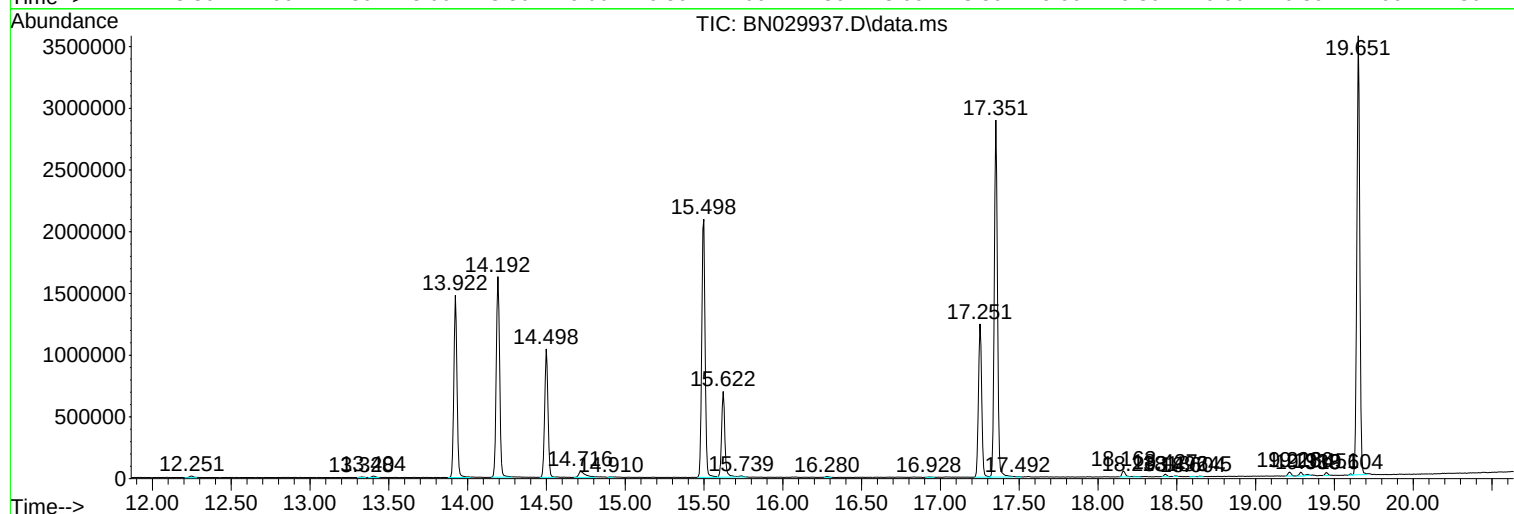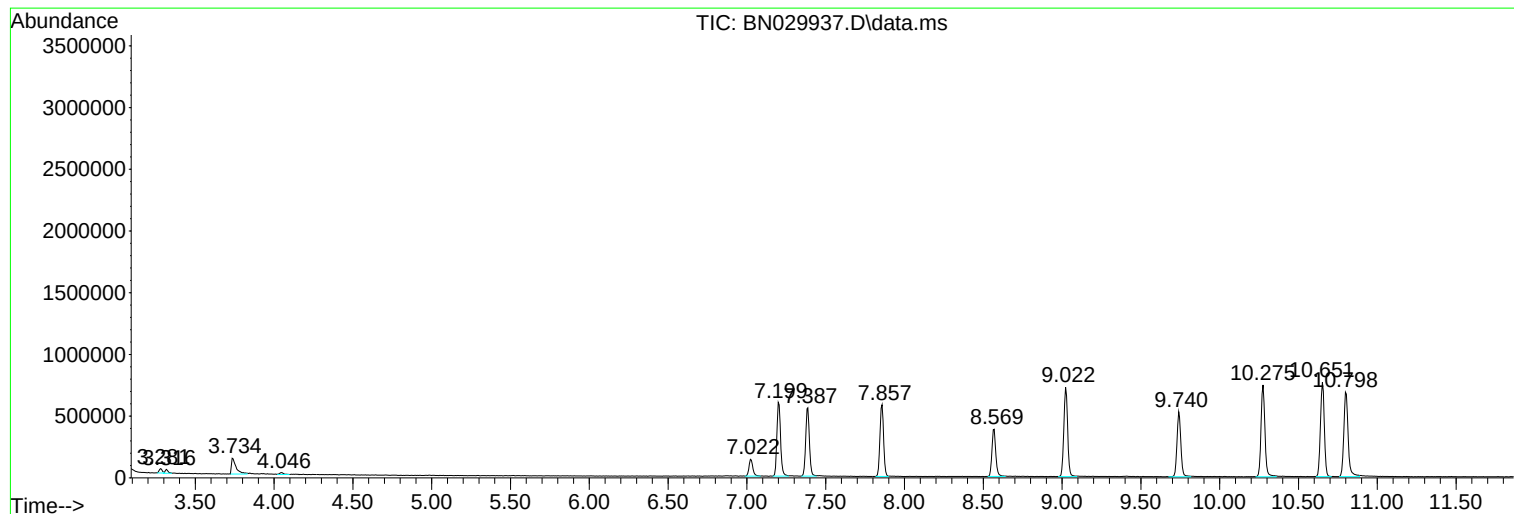

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029937.D
Acq On : 22 Feb 2024 21:03
Operator : MA/JU
Sample : P1494-04
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3Y6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029937.D
Acq On : 22 Feb 2024 21:03
Operator : MA/JU
Sample : P1494-04
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3Y6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc