

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
 Data File : BN029938.D
 Acq On : 22 Feb 2024 21:38
 Operator : MA/JU
 Sample : P1494-05
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH3Y5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029938.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.317	35	39	46	rVB	34712	47859	1.00%	0.112%
2	3.734	107	110	122	rBV	183455	325199	6.82%	0.759%
3	4.046	160	163	167	rVB2	15694	16997	0.36%	0.040%
4	6.863	637	642	643	rBV5	4356	6012	0.13%	0.014%
5	7.022	664	669	680	rVB	182063	301818	6.33%	0.704%
6	7.199	693	699	713	rBV	759219	1224188	25.66%	2.857%
7	7.387	723	731	742	rBV	724388	1173250	24.59%	2.738%
8	7.469	742	745	750	rVB6	4769	6707	0.14%	0.016%
9	7.857	804	811	820	rBV	562604	890815	18.67%	2.079%
10	8.563	925	931	944	rBV	508232	861185	18.05%	2.010%
11	9.022	1001	1009	1021	rBV	896230	1504508	31.54%	3.511%
12	9.134	1024	1028	1033	rVV4	6312	11034	0.23%	0.026%
13	9.740	1124	1131	1141	rBV	674243	1124062	23.56%	2.623%
14	10.275	1214	1222	1232	rBV	933782	1599042	33.52%	3.732%
15	10.651	1279	1286	1295	rVB	747887	1219303	25.56%	2.846%
16	10.798	1303	1311	1328	rBV	874163	1625535	34.07%	3.794%
17	11.469	1421	1425	1430	rBV6	2854	5684	0.12%	0.013%
18	12.245	1552	1557	1563	rBV	16004	25557	0.54%	0.060%
19	13.328	1737	1741	1745	rBV5	4453	6631	0.14%	0.015%
20	13.404	1749	1754	1760	rBV6	9283	15538	0.33%	0.036%
21	13.481	1760	1767	1768	rBV7	3152	5719	0.12%	0.013%
22	13.922	1835	1842	1853	rBV	1744968	2468144	51.74%	5.760%
23	14.192	1881	1888	1905	rBV2	2028075	2976919	62.40%	6.948%
24	14.498	1932	1940	1950	rBV	965549	1435872	30.10%	3.351%
25	14.716	1972	1977	1991	rBV2	51715	146828	3.08%	0.343%
26	14.928	2009	2013	2015	rBV5	4180	6129	0.13%	0.014%
27	15.498	2102	2110	2123	rBV	2520249	3715158	77.88%	8.671%
28	15.622	2125	2131	2144	rVV	735200	1057812	22.17%	2.469%
29	15.734	2147	2150	2158	rVB7	14736	24823	0.52%	0.058%
30	16.281	2239	2243	2249	rVB6	8110	12240	0.26%	0.029%
31	16.933	2349	2354	2357	rBV6	3689	4967	0.10%	0.012%
32	17.251	2402	2408	2418	rVV	1178586	1682416	35.27%	3.927%
33	17.351	2418	2425	2442	rVV	3012798	4294250	90.02%	10.022%
34	17.457	2442	2443	2448	rVB4	6530	5620	0.12%	0.013%
35	18.163	2557	2563	2571	rBV2	40981	66878	1.40%	0.156%
36	18.498	2616	2620	2627	rVB6	4168	8445	0.18%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029938.D
Acq On : 22 Feb 2024 21:38
Operator : MA/JU
Sample : P1494-05
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3Y5

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Title : SVOA CALIBRATION

37	19.216	2737	2742	2747	rBV2	32760	45719	0.96%	0.107%
38	19.286	2749	2754	2757	rBV	29883	42733	0.90%	0.100%
39	19.327	2759	2761	2765	rVB4	13936	15804	0.33%	0.037%
40	19.451	2778	2782	2788	rBV5	17246	24174	0.51%	0.056%
41	19.604	2805	2808	2810	rBV3	9574	11587	0.24%	0.027%
42	19.651	2810	2816	2824	rVV	3685326	4770505	100.00%	11.134%
43	21.186	3074	3077	3081	rBV4	22738	29017	0.61%	0.068%
44	21.451	3117	3122	3132	rBV2	1195520	1667971	34.96%	3.893%
45	23.662	3490	3498	3511	rBV	2302869	4591987	96.26%	10.717%
46	23.815	3517	3524	3535	rVB	827789	1744946	36.58%	4.072%




Sum of corrected areas: 42847587

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029938.D
Acq On : 22 Feb 2024 21:38
Operator : MA/JU
Sample : P1494-05
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3Y5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

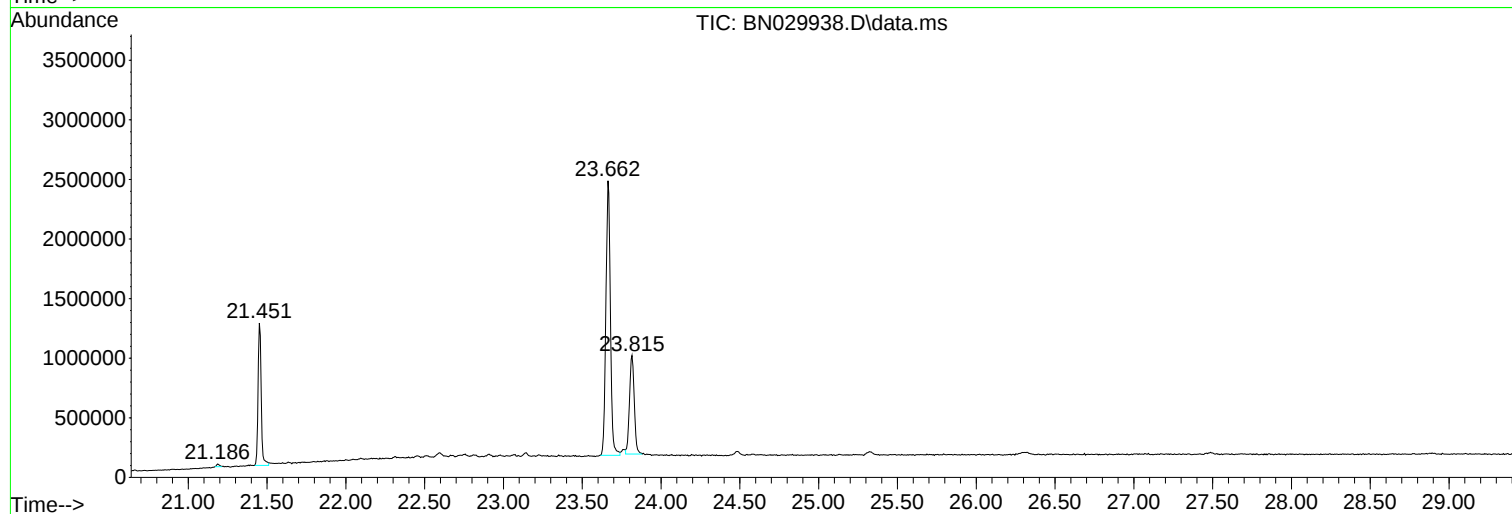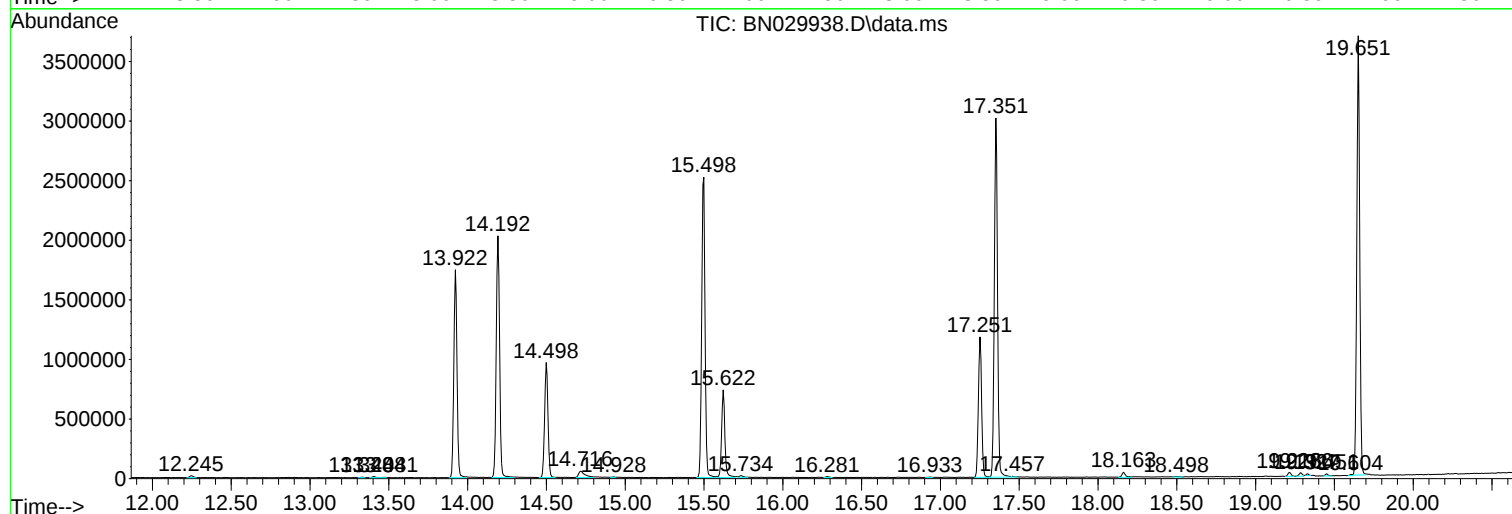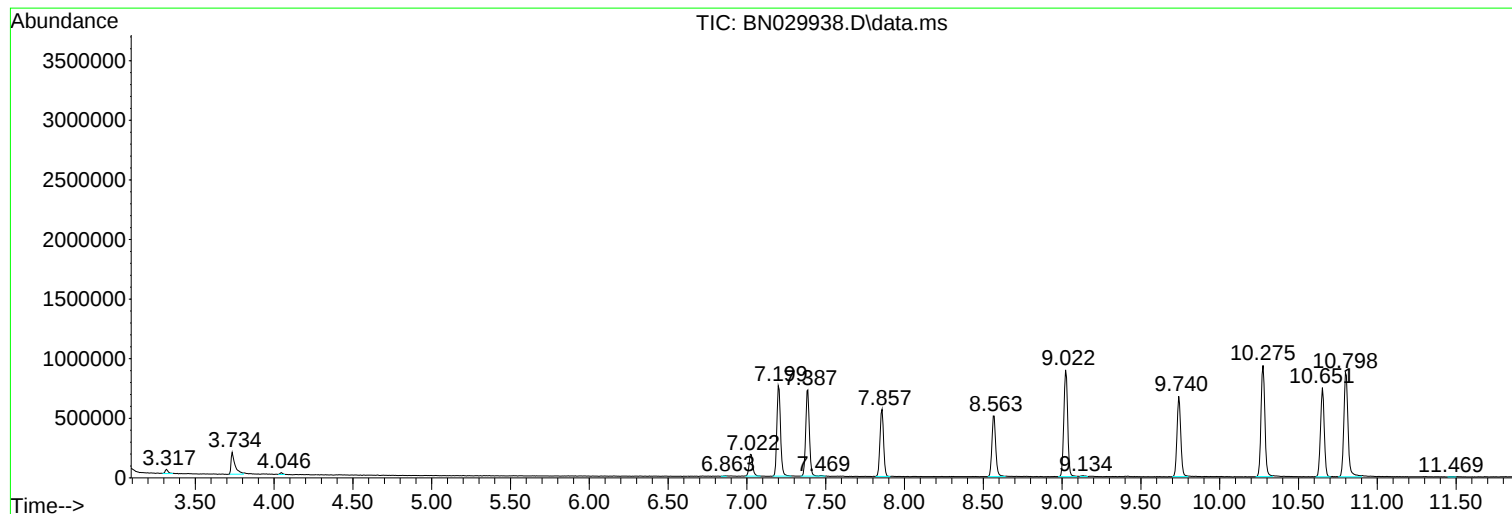

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029938.D
Acq On : 22 Feb 2024 21:38
Operator : MA/JU
Sample : P1494-05
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3Y5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029938.D
Acq On : 22 Feb 2024 21:38
Operator : MA/JU
Sample : P1494-05
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3Y5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc