

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
 Data File : BN029939.D
 Acq On : 22 Feb 2024 22:14
 Operator : MA/JU
 Sample : P1494-06
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH3Z8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029939.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.317	35	39	47	rVB	39462	50617	1.06%	0.117%
2	3.734	107	110	122	rBV	160234	298774	6.28%	0.688%
3	4.046	160	163	167	rVB2	13599	14592	0.31%	0.034%
4	7.022	663	669	683	rBV	238876	392590	8.25%	0.904%
5	7.199	693	699	713	rBV	804972	1294282	27.18%	2.979%
6	7.387	723	731	741	rBV	807820	1310315	27.52%	3.016%
7	7.858	803	811	819	rBV	557398	896409	18.83%	2.063%
8	8.563	923	931	942	rBV	605583	1007176	21.15%	2.318%
9	9.022	1002	1009	1019	rBV	962997	1578839	33.16%	3.634%
10	9.140	1023	1029	1034	rVV	37681	63971	1.34%	0.147%
11	9.740	1124	1131	1146	rBV	729945	1213380	25.49%	2.793%
12	10.140	1195	1199	1206	rBV7	5822	9839	0.21%	0.023%
13	10.275	1214	1222	1234	rBV	1006920	1712261	35.96%	3.941%
14	10.446	1249	1251	1258	rVB6	4590	5773	0.12%	0.013%
15	10.651	1276	1286	1294	rBV	723462	1206723	25.35%	2.778%
16	10.799	1303	1311	1332	rBV	851202	1582067	33.23%	3.642%
17	12.246	1551	1557	1562	rBV	15602	24624	0.52%	0.057%
18	13.328	1737	1741	1744	rBV6	3511	5047	0.11%	0.012%
19	13.404	1749	1754	1761	rVB2	18130	30220	0.63%	0.070%
20	13.469	1761	1765	1769	rBV5	3029	4841	0.10%	0.011%
21	13.740	1807	1811	1816	rBV7	3220	5956	0.13%	0.014%
22	13.922	1836	1842	1853	rBV	1768495	2479964	52.09%	5.709%
23	14.192	1881	1888	1902	rBV2	2081575	3050455	64.07%	7.022%
24	14.292	1902	1905	1911	rVB2	17269	28882	0.61%	0.066%
25	14.498	1933	1940	1951	rBV	940455	1391924	29.24%	3.204%
26	14.716	1968	1977	1990	rBV3	65756	181126	3.80%	0.417%
27	15.498	2102	2110	2125	rBV	2511067	3693535	77.58%	8.502%
28	15.622	2125	2131	2147	rVV	739129	1050283	22.06%	2.418%
29	15.734	2147	2150	2156	rVB6	11705	18661	0.39%	0.043%
30	16.063	2200	2206	2209	rBV6	3235	6506	0.14%	0.015%
31	16.281	2240	2243	2247	rVB4	8350	9993	0.21%	0.023%
32	17.251	2401	2408	2418	rBV	1152692	1640581	34.46%	3.776%
33	17.351	2418	2425	2442	rVV2	2916051	4207396	88.37%	9.685%
34	18.163	2559	2563	2569	rBV2	43928	60531	1.27%	0.139%
35	18.492	2615	2619	2623	rBV7	4309	6771	0.14%	0.016%
36	19.216	2737	2742	2748	rBV4	33016	49179	1.03%	0.113%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029939.D
Acq On : 22 Feb 2024 22:14
Operator : MA/JU
Sample : P1494-06
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3Z8

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Title : SVOA CALIBRATION

37	19.286	2749	2754	2758	rBV2	26492	41600	0.87%	0.096%
38	19.451	2778	2782	2789	rBV4	25455	37027	0.78%	0.085%
39	19.604	2805	2808	2810	rBV4	10661	11254	0.24%	0.026%
40	19.651	2810	2816	2831	rVB	3532666	4761097	100.00%	10.959%
41	21.186	3075	3077	3083	rVB6	18667	24896	0.52%	0.057%
42	21.451	3117	3122	3135	rBV2	1203369	1673081	35.14%	3.851%
43	23.668	3491	3499	3510	rBV2	2234312	4589337	96.39%	10.564%
44	23.815	3518	3524	3538	rVB	822462	1720284	36.13%	3.960%




Sum of corrected areas: 43442659

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029939.D
Acq On : 22 Feb 2024 22:14
Operator : MA/JU
Sample : P1494-06
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3Z8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

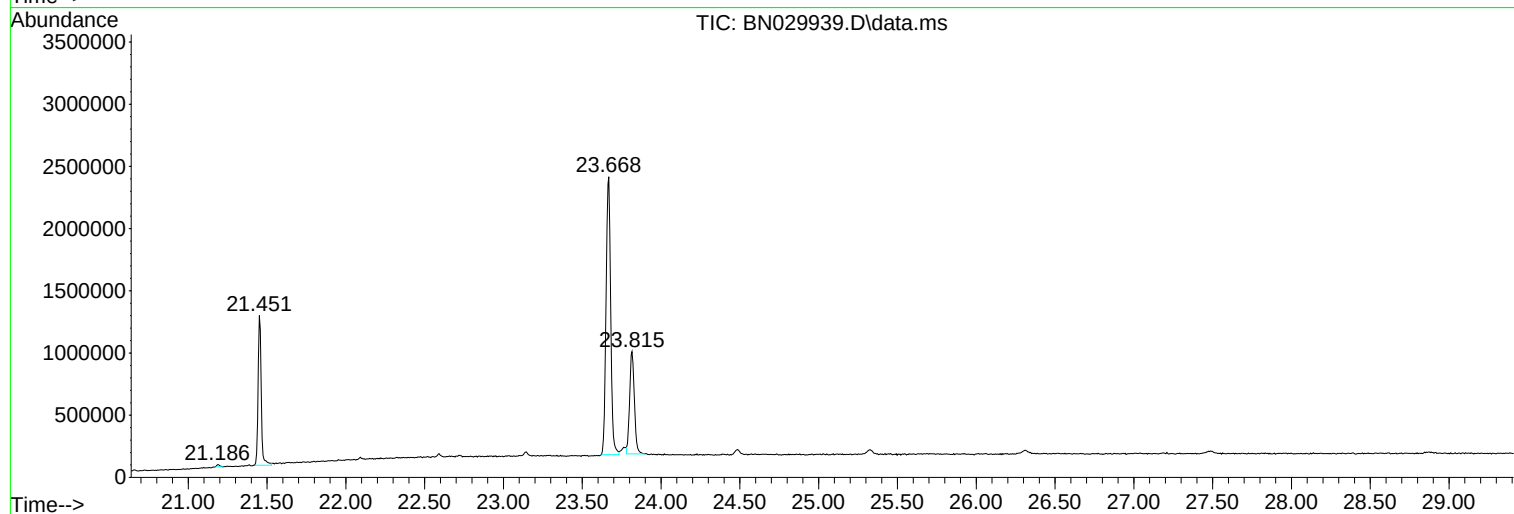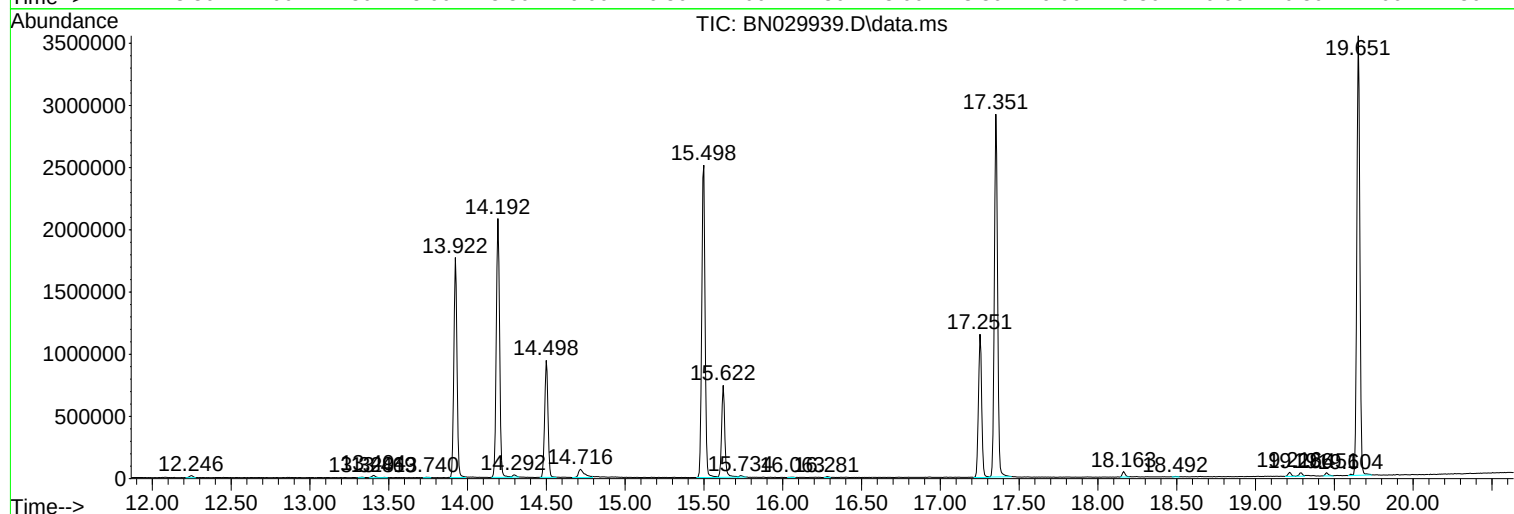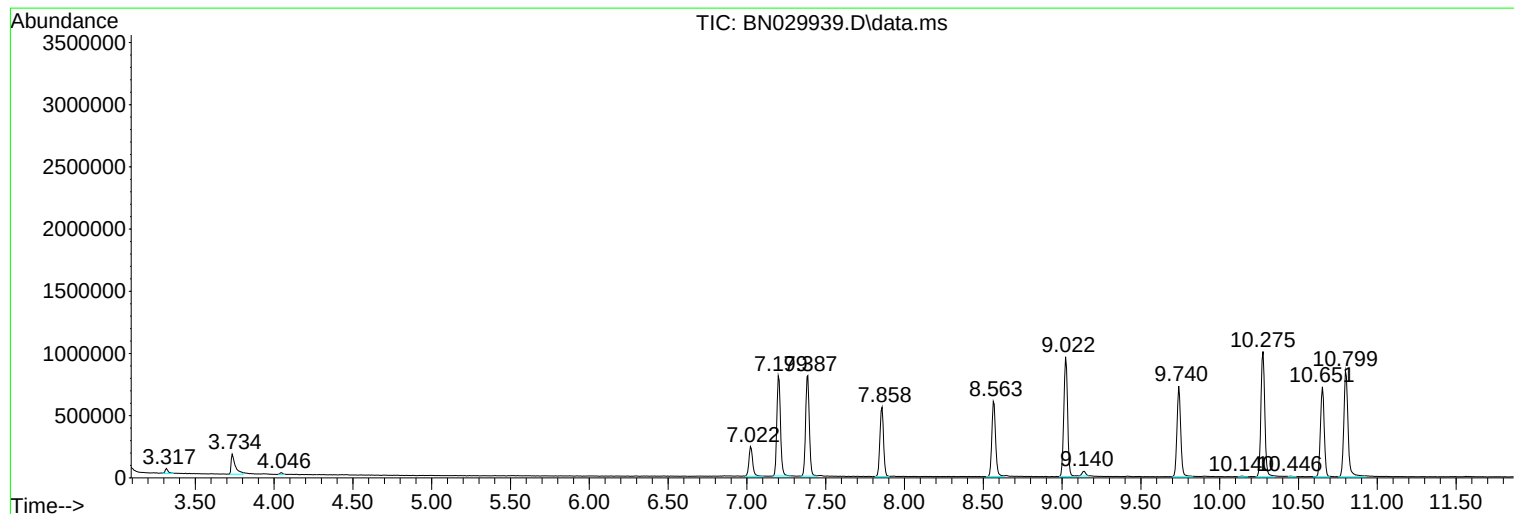

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029939.D
Acq On : 22 Feb 2024 22:14
Operator : MA/JU
Sample : P1494-06
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3Z8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029939.D
Acq On : 22 Feb 2024 22:14
Operator : MA/JU
Sample : P1494-06
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3Z8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc