

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
 Data File : BN029940.D
 Acq On : 22 Feb 2024 22:50
 Operator : MA/JU
 Sample : P1494-07
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH3Z9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029940.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.281	28	33	37	rBV	67149	96996	1.93%	0.227%
2	3.317	37	39	44	rVB	32700	36032	0.72%	0.085%
3	3.740	108	111	124	rBV	106063	215163	4.28%	0.505%
4	4.046	160	163	170	rVB2	15237	23072	0.46%	0.054%
5	6.869	638	643	646	rBV7	3635	6582	0.13%	0.015%
6	7.022	662	669	681	rVB	206508	338719	6.74%	0.794%
7	7.199	693	699	715	rVB	738754	1189768	23.66%	2.790%
8	7.381	723	730	742	rBV	717247	1168613	23.24%	2.741%
9	7.469	742	745	750	rVB7	4054	5528	0.11%	0.013%
10	7.858	801	811	818	rBV	516652	835432	16.61%	1.959%
11	8.563	924	931	945	rBV	541819	903666	17.97%	2.119%
12	9.022	1002	1009	1019	rBV	887299	1456342	28.96%	3.416%
13	9.134	1023	1028	1034	rVV2	13111	23234	0.46%	0.054%
14	9.416	1070	1076	1082	rVB7	5700	11371	0.23%	0.027%
15	9.740	1124	1131	1142	rBV	665914	1106513	22.00%	2.595%
16	10.275	1214	1222	1238	rBV	918865	1582348	31.47%	3.711%
17	10.652	1279	1286	1296	rVB	684120	1139344	22.66%	2.672%
18	10.799	1303	1311	1329	rBV	780838	1445071	28.74%	3.389%
19	12.246	1552	1557	1561	rBV3	15170	25054	0.50%	0.059%
20	12.463	1589	1594	1598	rBV8	2485	5141	0.10%	0.012%
21	13.334	1738	1742	1747	rVB7	5968	10982	0.22%	0.026%
22	13.404	1747	1754	1759	rBV2	15690	27210	0.54%	0.064%
23	13.922	1835	1842	1857	rBV	1708238	2363671	47.01%	5.544%
24	14.193	1881	1888	1899	rBV	1965569	2851723	56.71%	6.688%
25	14.298	1902	1906	1908	rVV5	4749	7156	0.14%	0.017%
26	14.498	1933	1940	1950	rBV	891467	1310186	26.06%	3.073%
27	14.716	1971	1977	1992	rBV2	66635	186567	3.71%	0.438%
28	15.498	2103	2110	2121	rBV	2372750	3490592	69.42%	8.186%
29	15.622	2124	2131	2146	rVV	786194	1123687	22.35%	2.635%
30	15.740	2147	2151	2155	rVB5	10257	16207	0.32%	0.038%
31	16.281	2238	2243	2247	rVB6	8200	11286	0.22%	0.026%
32	16.669	2305	2309	2315	rBV7	3274	7383	0.15%	0.017%
33	16.792	2327	2330	2335	rBV6	2897	5296	0.11%	0.012%
34	16.928	2350	2353	2358	rBB5	3677	5121	0.10%	0.012%
35	17.251	2402	2408	2417	rBV	1088024	1540502	30.64%	3.613%
36	17.351	2419	2425	2441	rVV2	2998576	4319672	85.90%	10.131%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
 Data File : BN029940.D
 Acq On : 22 Feb 2024 22:50
 Operator : MA/JU
 Sample : P1494-07
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH3Z9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

37	17.939	2521	2525	2527	rVB5	5265	5887	0.12%	0.014%
38	18.163	2557	2563	2570	rBV	86103	126227	2.51%	0.296%
39	19.216	2738	2742	2747	rVB3	34982	45503	0.90%	0.107%
40	19.286	2749	2754	2758	rBV	29626	46163	0.92%	0.108%
41	19.451	2777	2782	2788	rBV2	40254	60169	1.20%	0.141%
42	19.604	2805	2808	2810	rBV4	8383	7747	0.15%	0.018%
43	19.651	2810	2816	2825	rVV	3701295	4978852	99.01%	11.677%
44	19.916	2856	2861	2868	rVB	85579	104074	2.07%	0.244%
45	20.269	2918	2921	2924	rBV5	7793	8706	0.17%	0.020%
46	21.186	3074	3077	3086	rBV4	44622	70069	1.39%	0.164%
47	21.451	3117	3122	3136	rBV	1162331	1599635	31.81%	3.752%
48	23.663	3490	3498	3512	rBV2	2417907	5028487	100.00%	11.793%
49	23.816	3517	3524	3535	rVB	820017	1665655	33.12%	3.906%




Sum of corrected areas: 42638404

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029940.D
Acq On : 22 Feb 2024 22:50
Operator : MA/JU
Sample : P1494-07
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3Z9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

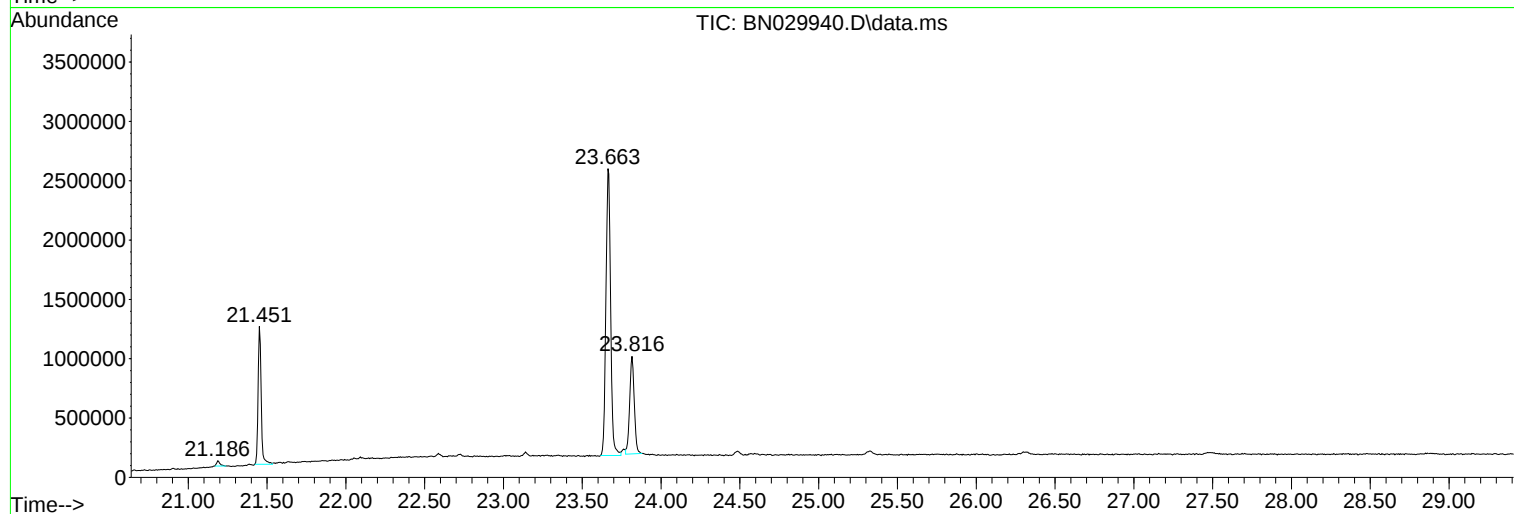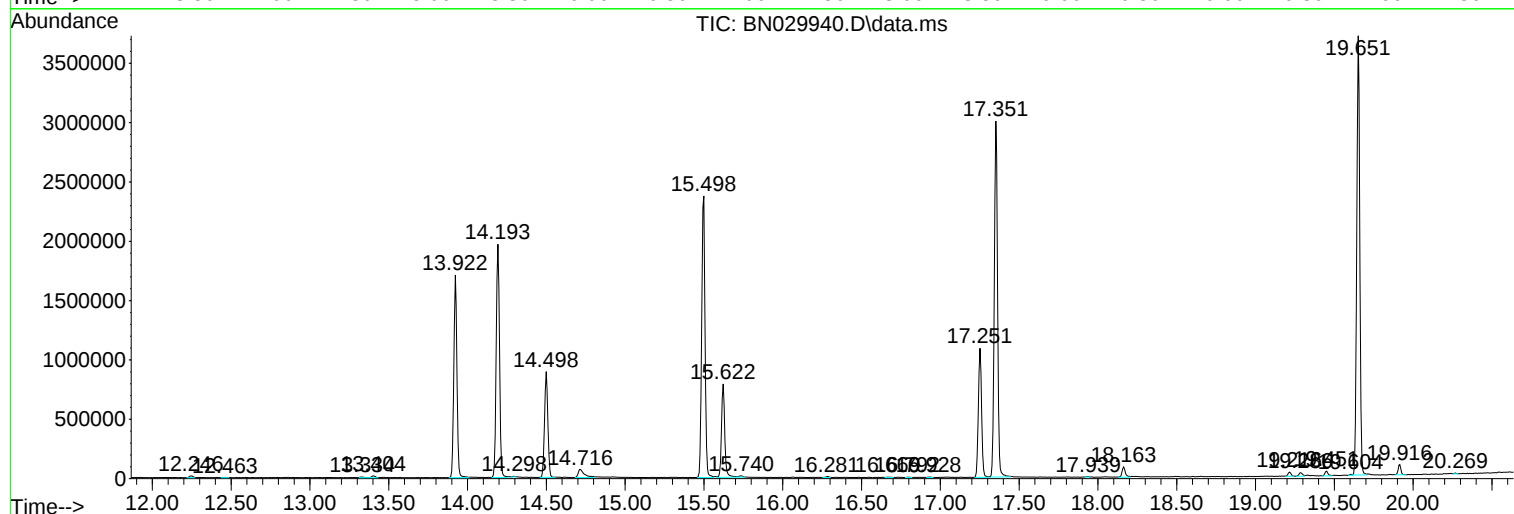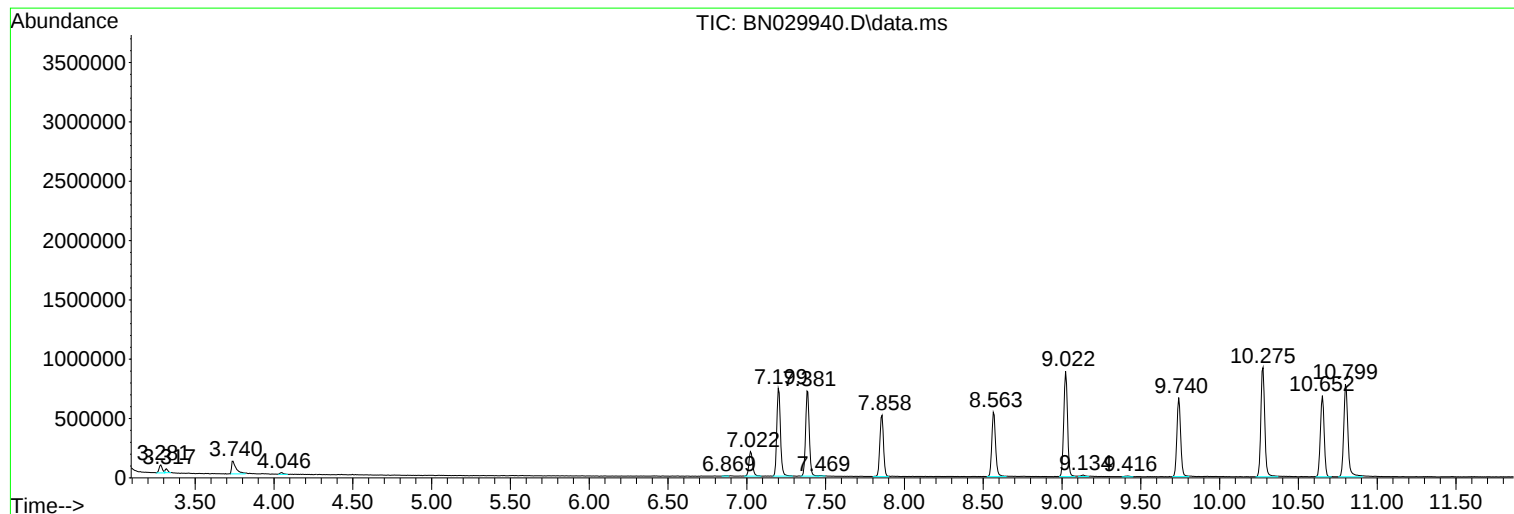

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029940.D
Acq On : 22 Feb 2024 22:50
Operator : MA/JU
Sample : P1494-07
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3Z9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029940.D
Acq On : 22 Feb 2024 22:50
Operator : MA/JU
Sample : P1494-07
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH3Z9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------