

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
 Data File : BN029941.D
 Acq On : 22 Feb 2024 23:26
 Operator : MA/JU
 Sample : P1455-01
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AA8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029941.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.281	27	33	55	rVB	1832367	2649065	55.99%	5.435%
2	3.734	107	110	124	rBV	220367	407374	8.61%	0.836%
3	4.046	159	163	170	rVB	21216	31747	0.67%	0.065%
4	4.569	246	252	261	rVB	374869	555451	11.74%	1.140%
5	5.228	361	364	369	rVB5	7159	9467	0.20%	0.019%
6	5.563	417	421	426	rVB6	4514	8765	0.19%	0.018%
7	7.022	663	669	679	rBV	224722	375708	7.94%	0.771%
8	7.199	692	699	712	rBV	830492	1333755	28.19%	2.737%
9	7.387	723	731	740	rBV	786724	1288782	27.24%	2.644%
10	7.469	743	745	748	rVB3	4549	5489	0.12%	0.011%
11	7.857	803	811	818	rBV	713935	1123878	23.75%	2.306%
12	8.563	925	931	942	rBV	573378	964096	20.38%	1.978%
13	9.022	1002	1009	1017	rBV	959396	1591859	33.64%	3.266%
14	9.416	1071	1076	1081	rVB3	7789	10804	0.23%	0.022%
15	9.740	1122	1131	1149	rBV	711408	1187891	25.10%	2.437%
16	10.275	1214	1222	1235	rBV	993273	1672525	35.35%	3.432%
17	10.651	1277	1286	1295	rBV	898426	1508440	31.88%	3.095%
18	10.798	1304	1311	1335	rBV	660144	1252276	26.47%	2.569%
19	12.245	1548	1557	1566	rVB2	17717	35112	0.74%	0.072%
20	12.851	1655	1660	1663	rBV7	2812	5078	0.11%	0.010%
21	13.404	1747	1754	1759	rBV4	12728	23752	0.50%	0.049%
22	13.922	1836	1842	1857	rBV	1805972	2561733	54.14%	5.256%
23	14.192	1879	1888	1909	rBV	2046567	3027998	63.99%	6.213%
24	14.498	1933	1940	1952	rBV	1168166	1735737	36.68%	3.561%
25	14.716	1971	1977	1987	rBV2	83399	199298	4.21%	0.409%
26	15.304	2074	2077	2081	rBV	11780	15874	0.34%	0.033%
27	15.498	2102	2110	2123	rBV	2470722	3714883	78.51%	7.622%
28	15.622	2125	2131	2140	rBV	728024	1012549	21.40%	2.078%
29	15.739	2146	2151	2156	rVB4	13269	22436	0.47%	0.046%
30	16.063	2203	2206	2210	rBV5	3093	4827	0.10%	0.010%
31	16.128	2212	2217	2226	rBV10	3430	10631	0.22%	0.022%
32	16.280	2239	2243	2248	rVB7	8530	14385	0.30%	0.030%
33	16.669	2300	2309	2312	rVB8	5428	13768	0.29%	0.028%
34	16.733	2316	2320	2324	rBV6	3113	5164	0.11%	0.011%
35	16.933	2350	2354	2357	rBV6	4094	5265	0.11%	0.011%
36	17.027	2367	2370	2375	rVB6	6273	10586	0.22%	0.022%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
 Data File : BN029941.D
 Acq On : 22 Feb 2024 23:26
 Operator : MA/JU
 Sample : P1455-01
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AA8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

37	17.133	2382	2388	2394	rVB9	4498	7286	0.15%	0.015%
38	17.251	2402	2408	2418	rBV	1451753	2031306	42.93%	4.168%
39	17.351	2418	2425	2449	rVB	2898138	4110834	86.88%	8.435%
40	17.557	2456	2460	2465	rVB6	4941	7460	0.16%	0.015%
41	17.933	2520	2524	2530	rVB6	18791	25747	0.54%	0.053%
42	18.163	2558	2563	2573	rBV	126569	185537	3.92%	0.381%
43	18.239	2574	2576	2581	rVB4	7443	11794	0.25%	0.024%
44	18.492	2616	2619	2623	rBV4	6941	10716	0.23%	0.022%
45	18.604	2635	2638	2640	rBV4	4409	4812	0.10%	0.010%
46	18.651	2642	2646	2649	rVB4	9022	13877	0.29%	0.028%
47	19.216	2738	2742	2746	rVB2	35329	43813	0.93%	0.090%
48	19.286	2749	2754	2760	rBV	32413	54364	1.15%	0.112%
49	19.451	2777	2782	2787	rBV2	79265	110412	2.33%	0.227%
50	19.604	2805	2808	2810	rBV3	16354	15067	0.32%	0.031%
51	19.651	2810	2816	2825	rVV	3523616	4731738	100.00%	9.709%
52	20.074	2886	2888	2890	rBV3	6137	5589	0.12%	0.011%
53	20.657	2985	2987	2990	rVB4	12692	12056	0.25%	0.025%
54	20.892	3025	3027	3032	rBV6	13117	22773	0.48%	0.047%
55	21.192	3074	3078	3084	rBV3	55388	85162	1.80%	0.175%
56	21.451	3117	3122	3132	rBV	1586693	2092985	44.23%	4.294%
57	23.662	3491	3498	3511	rBV2	2349022	4516000	95.44%	9.266%
58	23.815	3517	3524	3540	rVB	1075264	2240635	47.35%	4.597%




Sum of corrected areas: 48736411

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029941.D
Acq On : 22 Feb 2024 23:26
Operator : MA/JU
Sample : P1455-01
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AA8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

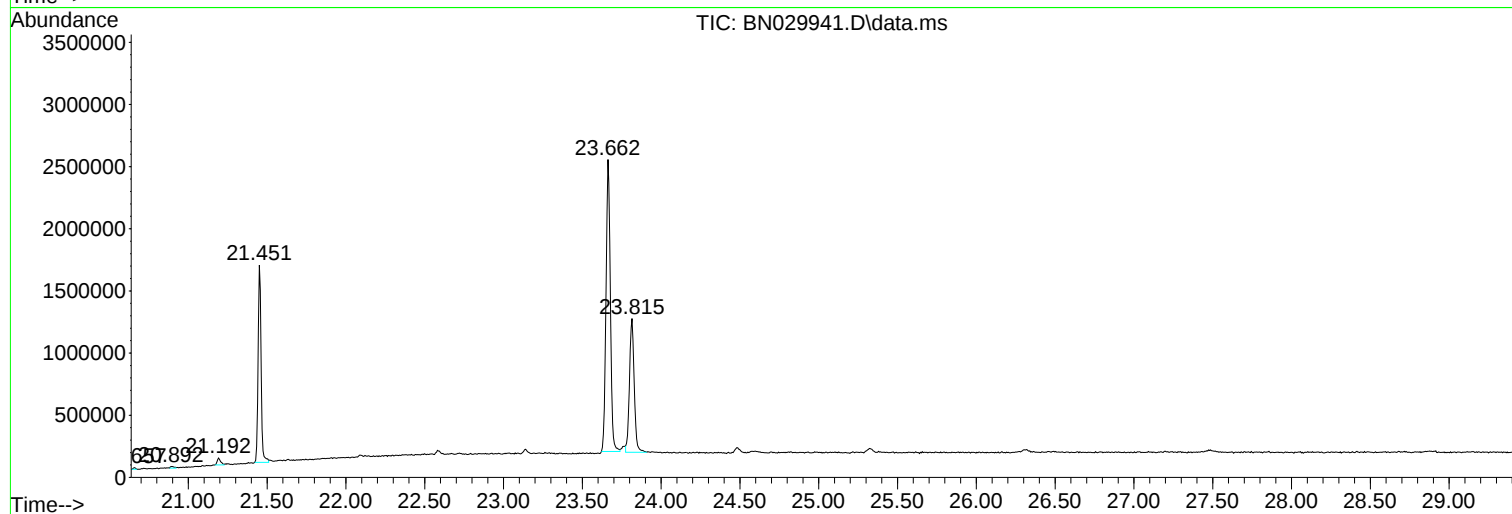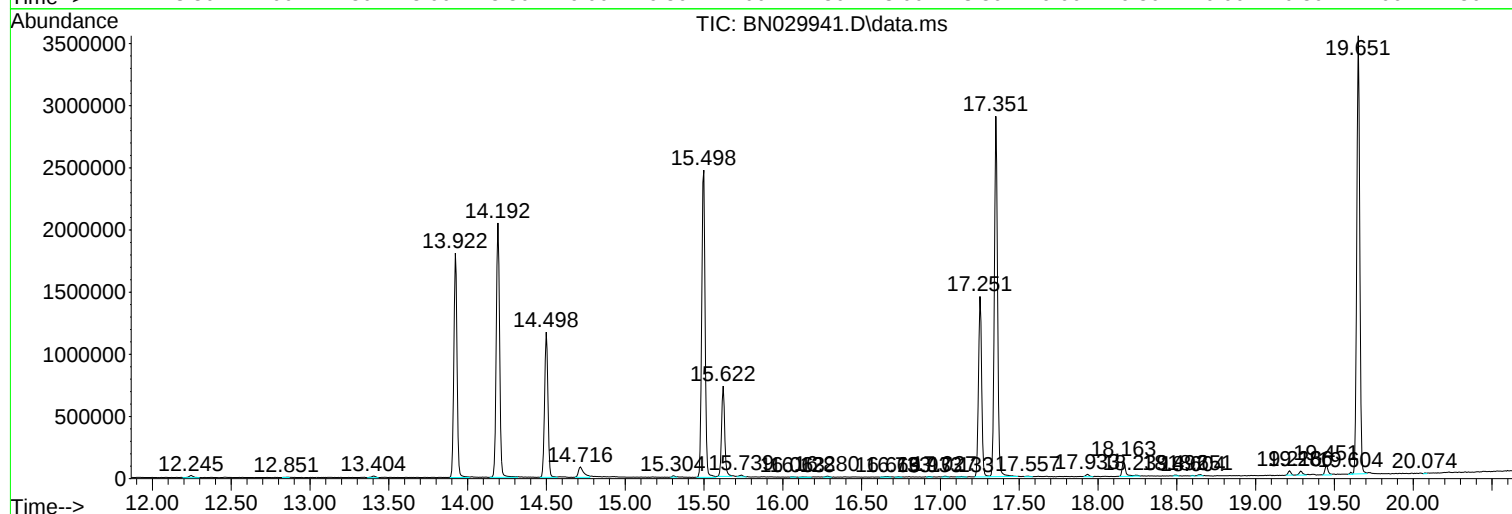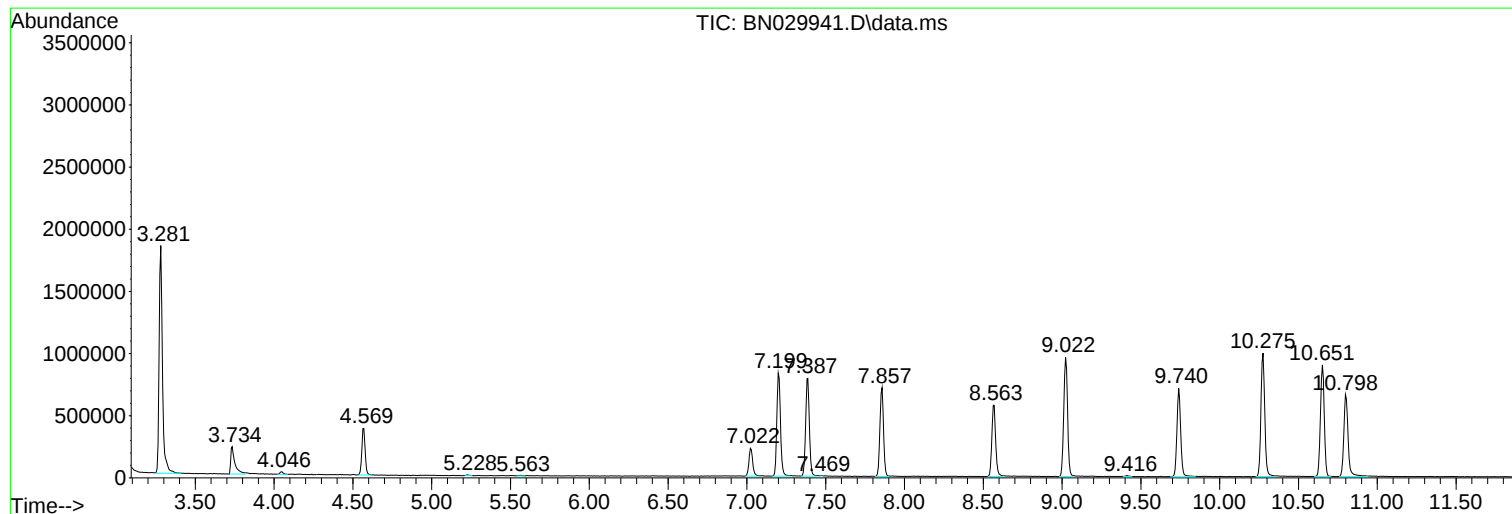

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029941.D
Acq On : 22 Feb 2024 23:26
Operator : MA/JU
Sample : P1455-01
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AA8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029941.D
Acq On : 22 Feb 2024 23:26
Operator : MA/JU
Sample : P1455-01
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AA8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------