

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
 Data File : BN029943.D
 Acq On : 23 Feb 2024 00:37
 Operator : MA/JU
 Sample : P1455-03
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AC5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029943.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.281	28	33	37	rBV	758586	1032989	21.38%	2.194%
2	3.740	108	111	126	rBV	100188	205761	4.26%	0.437%
3	4.046	160	163	168	rVB	17969	22562	0.47%	0.048%
4	4.570	246	252	259	rBV	303179	450737	9.33%	0.957%
5	7.022	664	669	682	rVB	244184	403344	8.35%	0.857%
6	7.199	692	699	714	rBV	874157	1397262	28.92%	2.968%
7	7.381	722	730	740	rBV	851642	1382891	28.62%	2.937%
8	7.469	742	745	749	rVB6	5356	8252	0.17%	0.018%
9	7.858	803	811	819	rBV	653587	1057487	21.89%	2.246%
10	8.563	925	931	950	rBV	636652	1063085	22.00%	2.258%
11	9.022	1000	1009	1020	rBV	1031524	1687666	34.93%	3.584%
12	9.410	1071	1075	1082	rVB3	6973	13302	0.28%	0.028%
13	9.740	1124	1131	1143	rBV	762132	1262812	26.14%	2.682%
14	10.275	1214	1222	1235	rBV	1057123	1811673	37.49%	3.848%
15	10.652	1279	1286	1295	rVB	852934	1430187	29.60%	3.038%
16	10.799	1304	1311	1325	rBV	474306	919858	19.04%	1.954%
17	12.251	1551	1558	1562	rBV2	18153	31589	0.65%	0.067%
18	12.457	1589	1593	1599	rVB6	3091	6956	0.14%	0.015%
19	13.410	1749	1755	1758	rBV4	7226	12414	0.26%	0.026%
20	13.922	1835	1842	1855	rBV	1931571	2654367	54.94%	5.638%
21	14.193	1881	1888	1900	rBV	2204203	3247622	67.21%	6.898%
22	14.498	1933	1940	1949	rBV	1110758	1629941	33.73%	3.462%
23	14.716	1969	1977	1990	rBV2	73203	195674	4.05%	0.416%
24	15.304	2073	2077	2082	rBV	16313	24912	0.52%	0.053%
25	15.498	2103	2110	2118	rBV	2624850	3931363	81.36%	8.350%
26	15.622	2125	2131	2147	rBV	752815	1074648	22.24%	2.282%
27	15.734	2147	2150	2158	rVB5	15211	24729	0.51%	0.053%
28	16.069	2201	2207	2211	rVB9	3830	7852	0.16%	0.017%
29	16.287	2240	2244	2247	rBV5	7315	11040	0.23%	0.023%
30	17.251	2400	2408	2418	rBV	1348198	1881286	38.94%	3.996%
31	17.351	2418	2425	2441	rVV2	3070013	4348678	90.00%	9.236%
32	17.934	2520	2524	2529	rVB8	6559	10568	0.22%	0.022%
33	18.163	2559	2563	2570	rBV	71407	101298	2.10%	0.215%
34	18.233	2572	2575	2579	rVV5	3692	6139	0.13%	0.013%
35	18.639	2642	2644	2651	rBV7	4274	6814	0.14%	0.014%
36	19.216	2737	2742	2747	rBV2	34629	45265	0.94%	0.096%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029943.D
Acq On : 23 Feb 2024 00:37
Operator : MA/JU
Sample : P1455-03
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC5

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Title : SVOA CALIBRATION

37	19.286	2749	2754	2759	rBV	33147	46738	0.97%	0.099%
38	19.445	2778	2781	2787	rBV3	33095	49828	1.03%	0.106%
39	19.604	2805	2808	2810	rBV3	10712	12049	0.25%	0.026%
40	19.651	2810	2816	2827	rVV	3580707	4831808	100.00%	10.262%
41	20.657	2985	2987	2993	rVB7	10529	10804	0.22%	0.023%
42	21.186	3074	3077	3085	rVB5	42077	71833	1.49%	0.153%
43	21.451	3117	3122	3132	rBV	1388180	1909818	39.53%	4.056%
44	23.663	3490	3498	3509	rBV	2363425	4723600	97.76%	10.032%
45	23.816	3517	3524	3536	rVB	967538	2024359	41.90%	4.299%




Sum of corrected areas: 47083860

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029943.D
Acq On : 23 Feb 2024 00:37
Operator : MA/JU
Sample : P1455-03
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

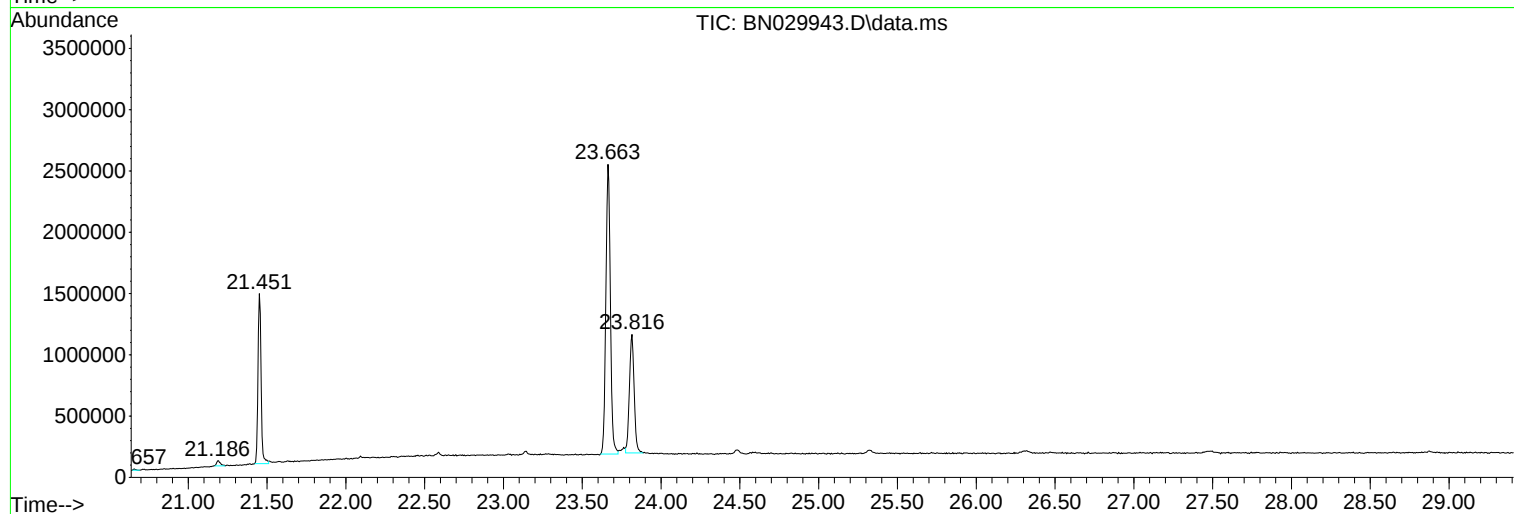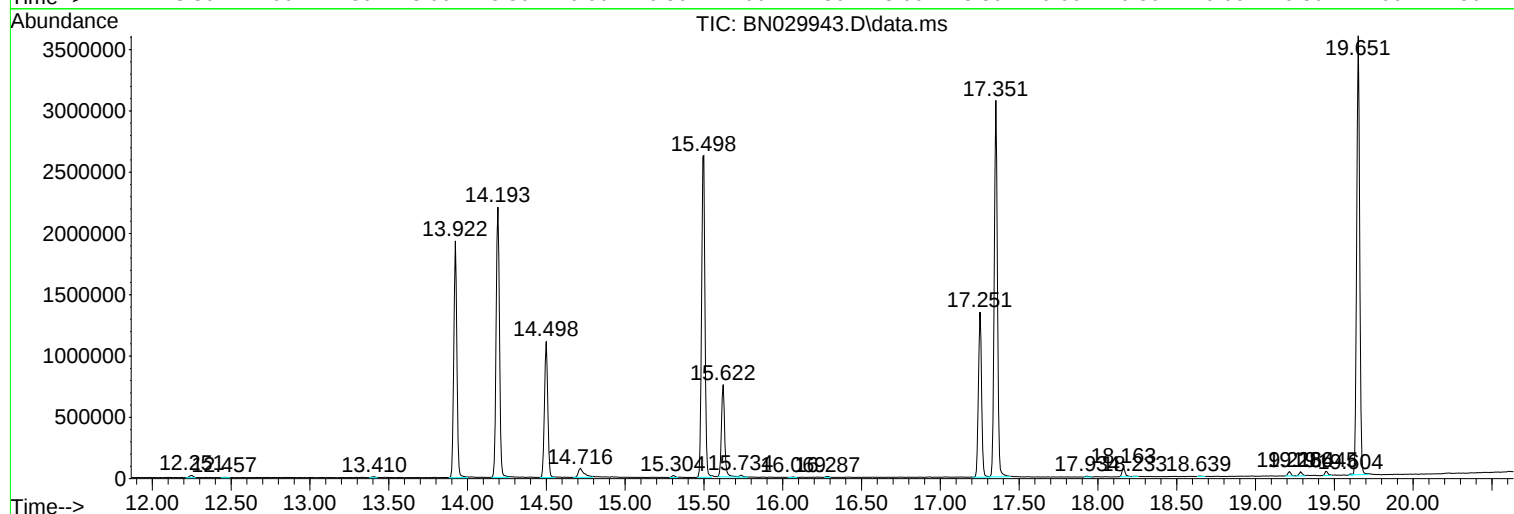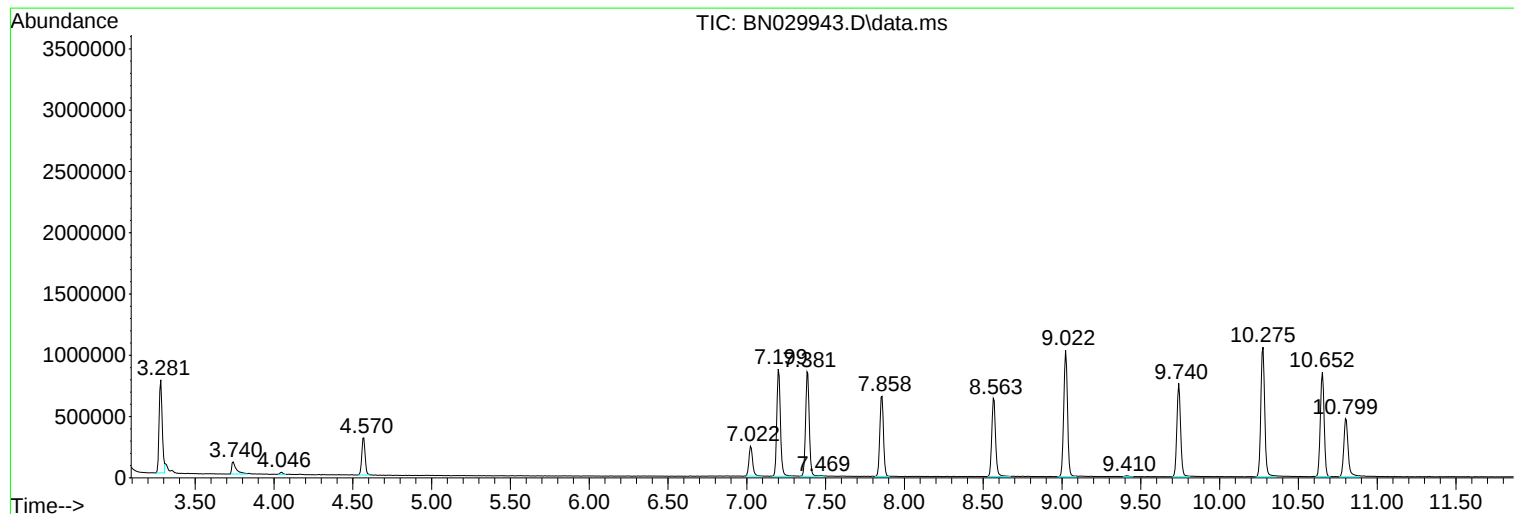

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029943.D
Acq On : 23 Feb 2024 00:37
Operator : MA/JU
Sample : P1455-03
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029943.D
Acq On : 23 Feb 2024 00:37
Operator : MA/JU
Sample : P1455-03
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AC5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc