

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
 Data File : BN029944.D
 Acq On : 23 Feb 2024 01:13
 Operator : MA/JU
 Sample : P1455-10
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AE3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029944.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.281	29	33	36	rBV	99975	130930	3.05%	0.319%
2	3.317	36	39	43	rVB	39141	45442	1.06%	0.111%
3	3.734	108	110	120	rBV	114715	214305	4.98%	0.522%
4	4.046	159	163	168	rBV	26650	33992	0.79%	0.083%
5	4.564	246	251	259	rVB	207172	308159	7.17%	0.751%
6	5.293	369	375	378	rBV6	2302	5020	0.12%	0.012%
7	7.022	663	669	681	rBV	220637	366920	8.53%	0.895%
8	7.199	693	699	715	rBV	826281	1313422	30.55%	3.202%
9	7.381	723	730	741	rBV	794717	1282074	29.82%	3.126%
10	7.858	803	811	822	rBV	524532	852050	19.82%	2.077%
11	8.563	923	931	947	rBV	591166	981286	22.83%	2.392%
12	8.746	959	962	969	rVB9	3734	6862	0.16%	0.017%
13	9.022	1000	1009	1022	rBV	965484	1587061	36.92%	3.869%
14	9.110	1022	1024	1032	rVB8	2863	6707	0.16%	0.016%
15	9.405	1071	1074	1084	rVB7	5481	10540	0.25%	0.026%
16	9.740	1122	1131	1144	rBV	689223	1155636	26.88%	2.817%
17	10.275	1214	1222	1238	rBV	961317	1655556	38.51%	4.036%
18	10.652	1278	1286	1299	rVB	672159	1130244	26.29%	2.756%
19	10.799	1303	1311	1336	rBV	802367	1513638	35.21%	3.690%
20	12.246	1552	1557	1563	rVB2	15892	25395	0.59%	0.062%
21	13.404	1749	1754	1759	rVB3	9045	15699	0.37%	0.038%
22	13.922	1835	1842	1853	rBV	1692233	2369928	55.13%	5.778%
23	14.193	1881	1888	1905	rBV	2031302	2954809	68.73%	7.204%
24	14.498	1933	1940	1949	rBV	894052	1290086	30.01%	3.145%
25	14.716	1969	1977	1989	rBV2	55644	153911	3.58%	0.375%
26	15.304	2071	2077	2081	rBV	12090	16002	0.37%	0.039%
27	15.498	2103	2110	2122	rBV	2341115	3515561	81.77%	8.571%
28	15.622	2125	2131	2143	rVV	645181	908622	21.13%	2.215%
29	15.734	2146	2150	2154	rVB6	10406	16066	0.37%	0.039%
30	16.069	2200	2207	2211	rBV9	2865	5162	0.12%	0.013%
31	16.204	2225	2230	2233	rBV7	2916	5139	0.12%	0.013%
32	16.287	2239	2244	2247	rBV6	7139	9314	0.22%	0.023%
33	17.251	2401	2408	2418	rBV	1072636	1491697	34.70%	3.637%
34	17.351	2418	2425	2444	rVB2	2748980	3905320	90.84%	9.521%
35	17.551	2457	2459	2464	rBV6	3751	4575	0.11%	0.011%
36	18.163	2557	2563	2571	rVV3	28386	45342	1.05%	0.111%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029944.D
Acq On : 23 Feb 2024 01:13
Operator : MA/JU
Sample : P1455-10
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AE3

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Title : SVOA CALIBRATION

37	19.216	2738	2742	2749	rVB2	32577	46801	1.09%	0.114%
38	19.286	2749	2754	2760	rBV	27844	47365	1.10%	0.115%
39	19.451	2778	2782	2786	rBV6	14070	17822	0.41%	0.043%
40	19.604	2805	2808	2810	rBV3	10578	12892	0.30%	0.031%
41	19.651	2810	2816	2824	rVV	3219334	4299146	100.00%	10.481%
42	21.451	3117	3122	3139	rBV	1123068	1534004	35.68%	3.740%
43	23.663	3491	3498	3509	rBV2	2031088	4121452	95.87%	10.048%
44	23.816	3518	3524	3545	rVB	767357	1605369	37.34%	3.914%




Sum of corrected areas: 41017323

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029944.D
Acq On : 23 Feb 2024 01:13
Operator : MA/JU
Sample : P1455-10
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AE3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

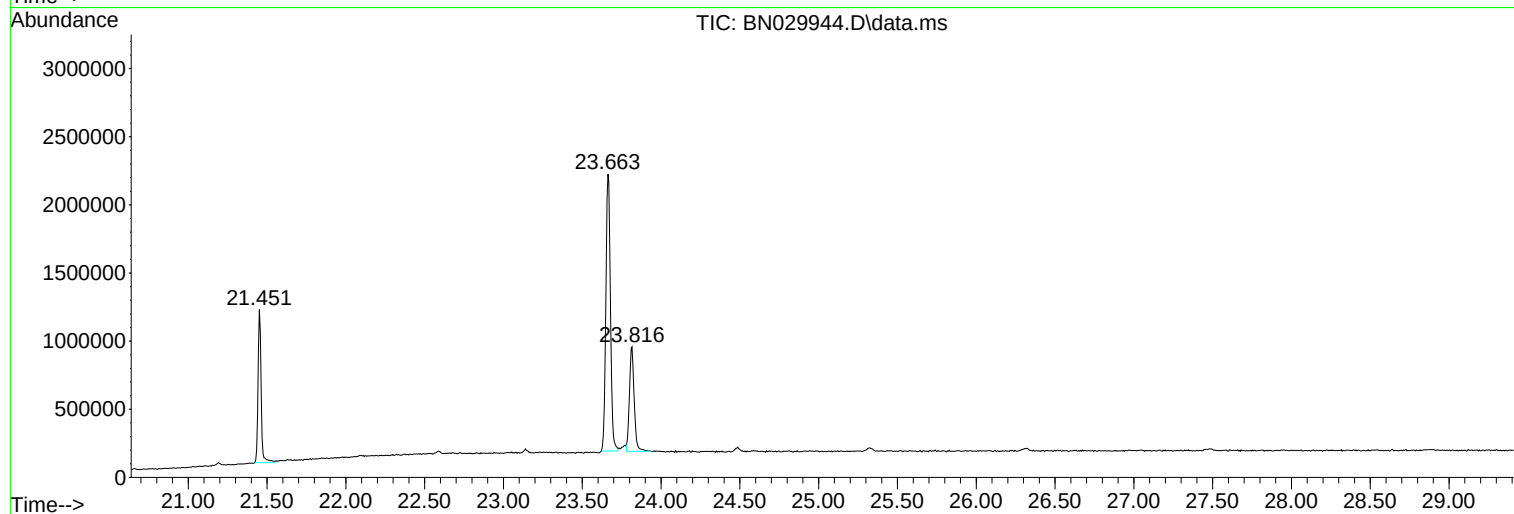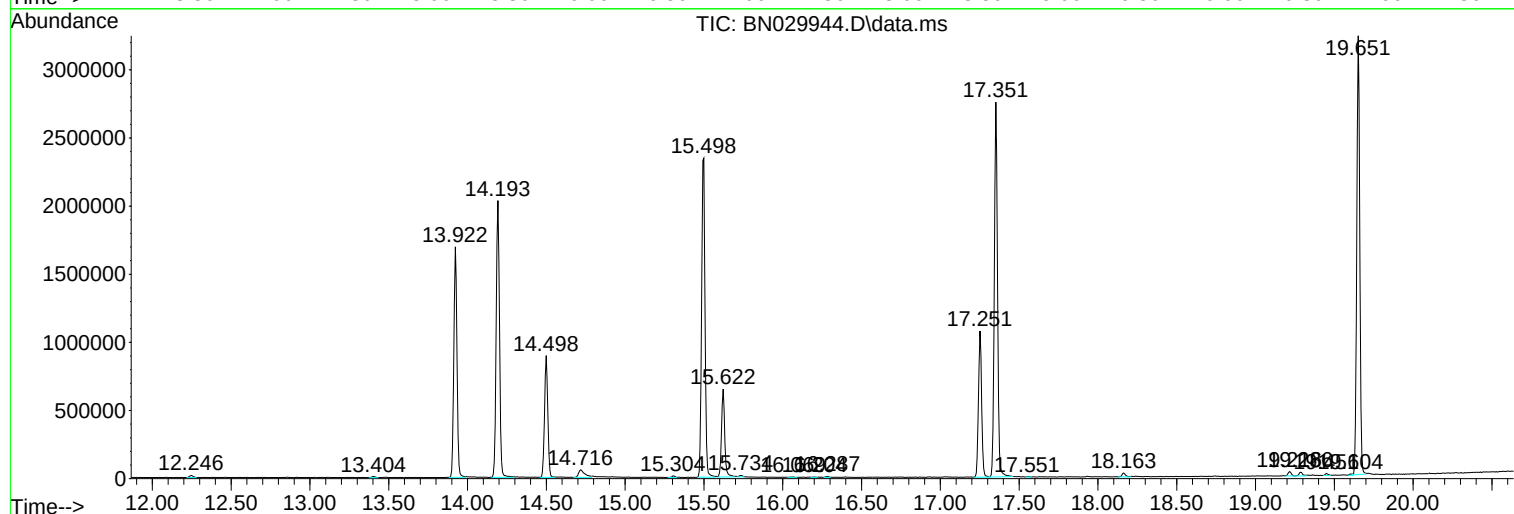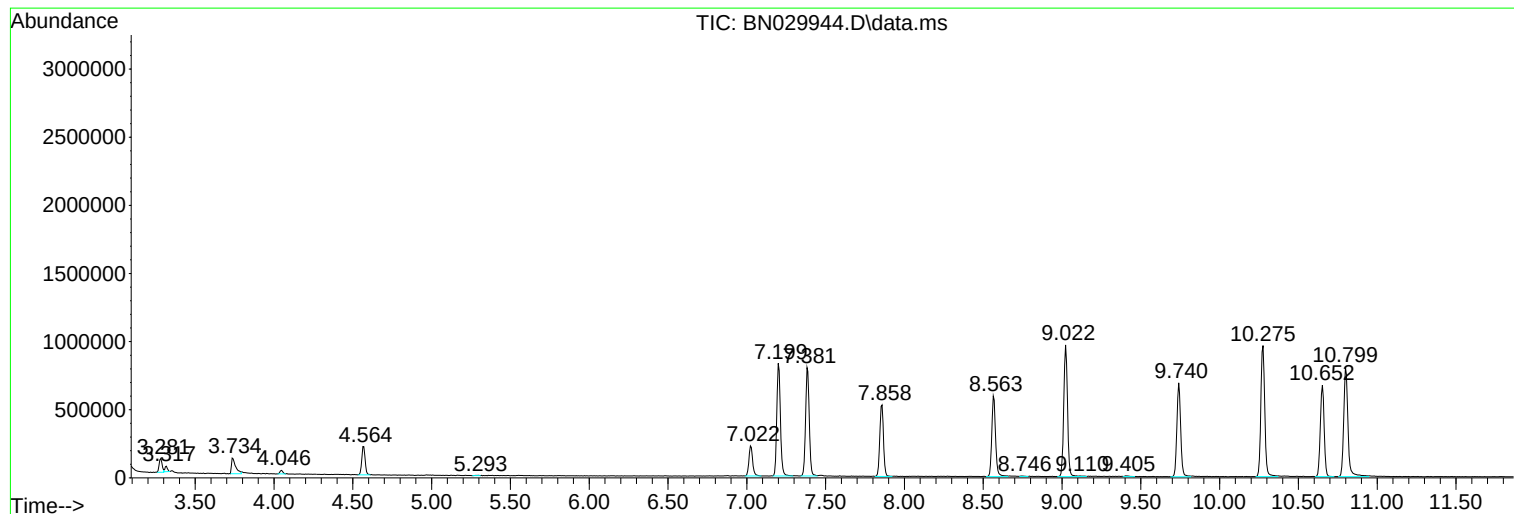

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029944.D
Acq On : 23 Feb 2024 01:13
Operator : MA/JU
Sample : P1455-10
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AE3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029944.D
Acq On : 23 Feb 2024 01:13
Operator : MA/JU
Sample : P1455-10
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AE3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------