

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
 Data File : BN029949.D
 Acq On : 23 Feb 2024 09:05
 Operator : MA/JU
 Sample : PB159158BL
 Misc :
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK158

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029949.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.305	33	37	46	rVB	102918	135244	2.21%	0.187%
2	3.710	103	106	124	rBV	1118197	1812543	29.67%	2.505%
3	4.028	155	160	168	rVB3	46920	81523	1.33%	0.113%
4	4.204	186	190	194	rBV6	9964	15302	0.25%	0.021%
5	4.257	195	199	209	rBV3	40018	61227	1.00%	0.085%
6	4.410	221	225	232	rVB4	16561	25745	0.42%	0.036%
7	4.593	251	256	261	rVB	67126	92873	1.52%	0.128%
8	4.640	261	264	267	rBV	24095	37143	0.61%	0.051%
9	5.740	447	451	457	rVB7	10656	17394	0.28%	0.024%
10	5.804	457	462	465	rBV7	4196	6605	0.11%	0.009%
11	6.151	519	521	529	rVB6	5694	11890	0.19%	0.016%
12	6.640	600	604	607	rBV6	3754	6470	0.11%	0.009%
13	7.010	659	667	686	rBV	1425030	2322847	38.03%	3.211%
14	7.187	690	697	715	rVB	1142266	1811697	29.66%	2.504%
15	7.369	720	728	736	rBV	1487538	2321218	38.00%	3.209%
16	7.545	753	758	763	rVB8	8037	13931	0.23%	0.019%
17	7.840	801	808	816	rVB	1091705	1691646	27.69%	2.338%
18	8.004	832	836	840	rBV5	4440	6962	0.11%	0.010%
19	8.087	843	850	854	rBV5	8068	15490	0.25%	0.021%
20	8.551	922	929	944	rBV	1701419	2708431	44.34%	3.744%
21	8.816	970	974	978	rBV7	4551	8892	0.15%	0.012%
22	9.010	999	1007	1019	rBV	1347560	2213274	36.23%	3.059%
23	9.175	1033	1035	1042	rVB6	3873	6676	0.11%	0.009%
24	9.728	1119	1129	1142	rBV	1079751	1790271	29.31%	2.475%
25	9.998	1169	1175	1177	rBV6	4031	6540	0.11%	0.009%
26	10.263	1212	1220	1236	rBV	1549745	2701306	44.22%	3.734%
27	10.504	1257	1261	1267	rVB8	5099	8492	0.14%	0.012%
28	10.639	1276	1284	1292	rBV	1419520	2376174	38.90%	3.285%
29	10.786	1301	1309	1326	rBV	1474057	2670111	43.71%	3.691%
30	11.298	1390	1396	1397	rBV6	7472	11933	0.20%	0.016%
31	11.322	1397	1400	1406	rVB5	8450	12990	0.21%	0.018%
32	11.404	1409	1414	1418	rVB5	5981	9558	0.16%	0.013%
33	12.092	1526	1531	1541	rBV5	2783	6987	0.11%	0.010%
34	12.233	1549	1555	1560	rBV2	28906	46783	0.77%	0.065%
35	13.398	1748	1753	1758	rBV	22431	37725	0.62%	0.052%
36	13.916	1834	1841	1853	rBV	2523791	3475776	56.90%	4.805%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
 Data File : BN029949.D
 Acq On : 23 Feb 2024 09:05
 Operator : MA/JU
 Sample : PB159158BL
 Misc :
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK158

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

37	14.186	1877	1887	1900	rBV	2862913	4292734	70.27%	5.934%
38	14.492	1932	1939	1949	rVB	1925776	2797358	45.79%	3.867%
39	14.704	1968	1975	1998	rBV	896590	1674481	27.41%	2.315%
40	14.857	1998	2001	2004	rVB5	5277	7279	0.12%	0.010%
41	15.163	2050	2053	2059	rVB6	4836	7956	0.13%	0.011%
42	15.274	2065	2072	2077	rBV7	4630	10139	0.17%	0.014%
43	15.433	2090	2099	2102	rBV4	17438	39843	0.65%	0.055%
44	15.492	2102	2109	2120	rVV	3529722	5071880	83.03%	7.011%
45	15.616	2123	2130	2145	rVV	1022057	1472450	24.10%	2.035%
46	15.727	2145	2149	2154	rVB4	14591	23944	0.39%	0.033%
47	15.910	2175	2180	2185	rBV3	13539	22619	0.37%	0.031%
48	16.057	2199	2205	2207	rVB6	5055	8835	0.14%	0.012%
49	16.122	2211	2216	2219	rVB3	5297	9805	0.16%	0.014%
50	16.274	2238	2242	2247	rVB4	12244	18780	0.31%	0.026%
51	16.551	2286	2289	2296	rBV6	6502	15024	0.25%	0.021%
52	16.721	2313	2318	2325	rBV	30277	51815	0.85%	0.072%
53	16.921	2350	2352	2357	rVB5	4988	6343	0.10%	0.009%
54	17.033	2365	2371	2377	rBV7	6387	13016	0.21%	0.018%
55	17.104	2377	2383	2387	rBV	11577	18717	0.31%	0.026%
56	17.245	2401	2407	2417	rBV	2193548	3272811	53.58%	4.524%
57	17.351	2417	2425	2445	rVB	3859231	5471537	89.57%	7.563%
58	17.663	2475	2478	2483	rBV5	7771	9276	0.15%	0.013%
59	17.804	2498	2502	2505	rBV	20401	24487	0.40%	0.034%
60	17.927	2514	2523	2526	rBV10	6584	14576	0.24%	0.020%
61	18.151	2553	2561	2569	rBV6	15601	35255	0.58%	0.049%
62	18.304	2584	2587	2592	rVB7	4813	8610	0.14%	0.012%
63	18.492	2615	2619	2622	rVB5	5448	8776	0.14%	0.012%
64	18.651	2642	2646	2650	rBV6	9116	14832	0.24%	0.021%
65	18.698	2650	2654	2657	rVV6	8695	11690	0.19%	0.016%
66	18.757	2657	2664	2669	rVV2	19658	28920	0.47%	0.040%
67	19.068	2715	2717	2723	rVB4	5862	9412	0.15%	0.013%
68	19.215	2737	2742	2749	rVB2	43901	66222	1.08%	0.092%
69	19.286	2749	2754	2764	rBV2	39784	73570	1.20%	0.102%
70	19.363	2764	2767	2771	rVV4	13316	15538	0.25%	0.021%
71	19.451	2779	2782	2786	rBV5	6279	10052	0.16%	0.014%
72	19.568	2798	2802	2804	rBV2	15460	17750	0.29%	0.025%
73	19.604	2804	2808	2810	rBV2	38713	42520	0.70%	0.059%
74	19.651	2810	2816	2825	rVB	4489267	6108607	100.00%	8.444%
75	19.874	2851	2854	2859	rVB4	13985	14645	0.24%	0.020%
76	20.268	2919	2921	2926	rVB2	22318	22282	0.36%	0.031%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029949.D
Acq On : 23 Feb 2024 09:05
Operator : MA/JU
Sample : PB159158BL
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK158

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Title : SVOA CALIBRATION

77	20.662	2984	2988	2993	rBV2	33829	44594	0.73%	0.062%
78	20.909	3026	3030	3036	rBV4	23864	35346	0.58%	0.049%
79	21.162	3070	3073	3076	rBV2	44252	46747	0.77%	0.065%
80	21.457	3117	3123	3134	rBV2	2439013	3362236	55.04%	4.648%
81	23.151	3408	3411	3418	rVB4	75927	113793	1.86%	0.157%
82	23.674	3491	3500	3511	rBV2	2884808	5950981	97.42%	8.226%
83	23.821	3519	3525	3539	rVB2	1652421	3366361	55.11%	4.653%




Sum of corrected areas: 72344113

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029949.D
Acq On : 23 Feb 2024 09:05
Operator : MA/JU
Sample : PB159158BL
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK158

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

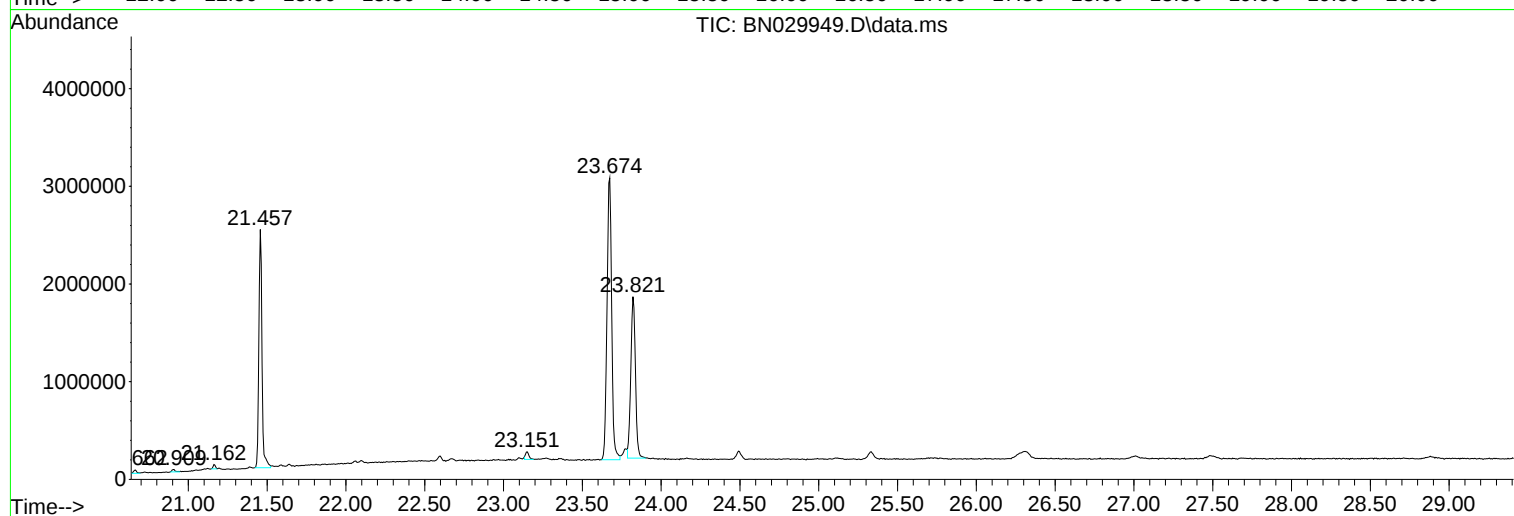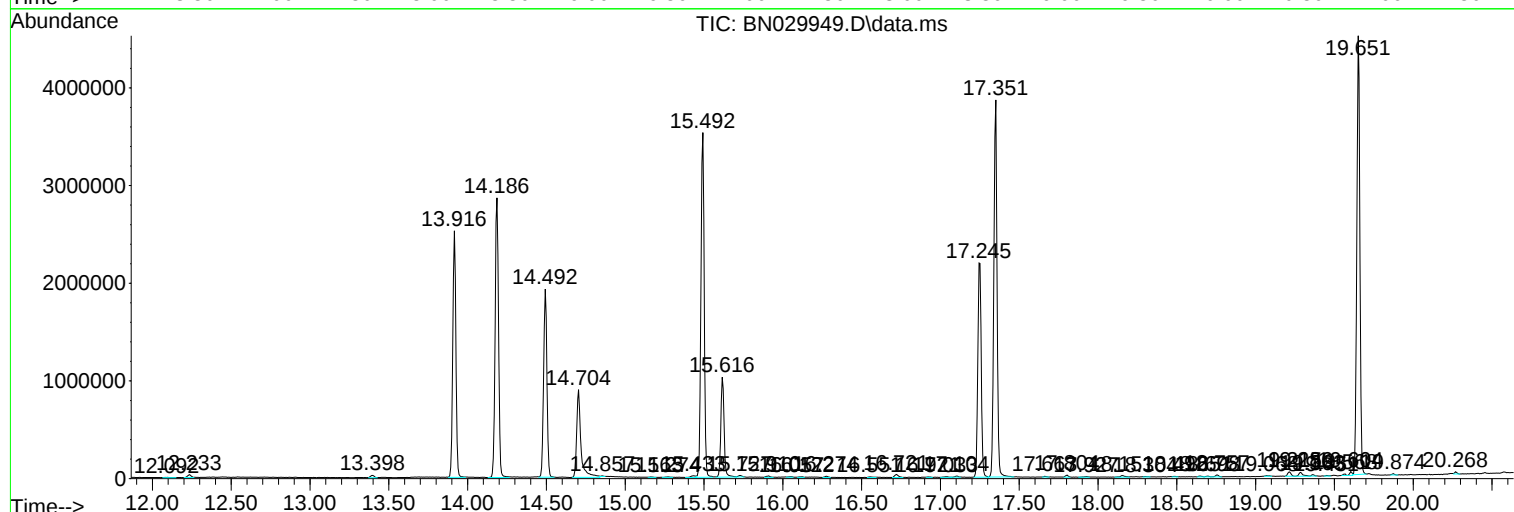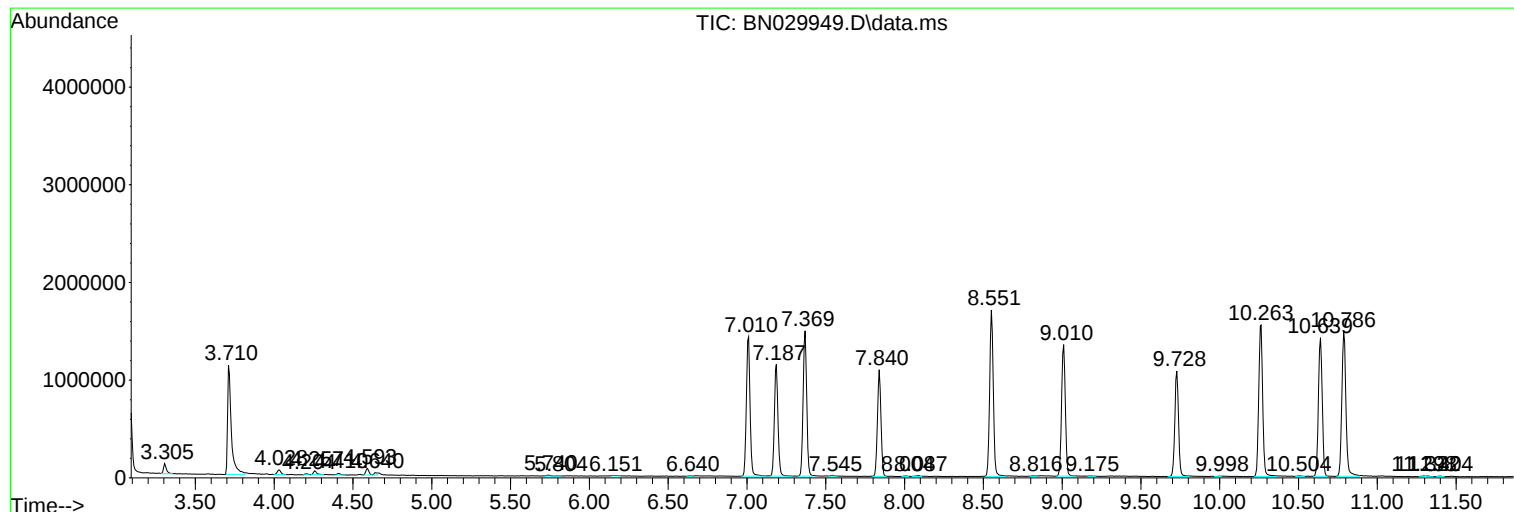

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029949.D
Acq On : 23 Feb 2024 09:05
Operator : MA/JU
Sample : PB159158BL
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK158

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029949.D
Acq On : 23 Feb 2024 09:05
Operator : MA/JU
Sample : PB159158BL
Misc :
ALS Vial : 71 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK158

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------