

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
 Data File : BN029950.D
 Acq On : 23 Feb 2024 09:41
 Operator : MA/JU
 Sample : P1455-10
 Misc :
 ALS Vial : 72 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AE3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029950.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.276	28	32	36	rBV	107284	148314	3.01%	0.310%
2	3.311	36	38	43	rVB	39281	48140	0.98%	0.101%
3	3.734	107	110	127	rBV	130458	252627	5.12%	0.528%
4	4.046	159	163	171	rVB	29524	41021	0.83%	0.086%
5	4.564	246	251	260	rVB	231679	333631	6.76%	0.697%
6	7.022	662	669	682	rBV	236041	401293	8.13%	0.839%
7	7.199	692	699	708	rBV	889190	1414544	28.67%	2.957%
8	7.381	723	730	741	rBV	878875	1383297	28.03%	2.891%
9	7.469	741	745	747	rVB5	5739	7993	0.16%	0.017%
10	7.852	803	810	819	rBV	679795	1080201	21.89%	2.258%
11	8.563	923	931	941	rBV	660929	1064571	21.58%	2.225%
12	9.016	1001	1008	1018	rBV	1031880	1725407	34.97%	3.607%
13	9.410	1071	1075	1079	rBV5	5403	7170	0.15%	0.015%
14	9.734	1122	1130	1142	rBV	743890	1289500	26.13%	2.695%
15	10.269	1213	1221	1233	rBV	1072441	1837237	37.23%	3.840%
16	10.646	1278	1285	1293	rVB	886493	1493965	30.28%	3.123%
17	10.799	1303	1311	1332	rBV	885051	1681427	34.08%	3.515%
18	12.246	1552	1557	1562	rBV	18122	31171	0.63%	0.065%
19	13.404	1750	1754	1759	rVB5	6298	10287	0.21%	0.022%
20	13.922	1834	1842	1854	rBV	1865169	2675199	54.22%	5.592%
21	14.193	1878	1888	1897	rBV	2154496	3301414	66.91%	6.901%
22	14.398	1920	1923	1928	rVB6	3326	5200	0.11%	0.011%
23	14.498	1932	1940	1952	rBV	1182984	1774041	35.95%	3.708%
24	14.716	1970	1977	1989	rBV2	59684	176894	3.59%	0.370%
25	15.304	2072	2077	2083	rBV4	11921	21538	0.44%	0.045%
26	15.493	2102	2109	2124	rBV	2754917	4026935	81.61%	8.417%
27	15.622	2124	2131	2145	rVV	691654	1068607	21.66%	2.234%
28	15.734	2147	2150	2157	rVB3	13671	22469	0.46%	0.047%
29	16.181	2220	2226	2228	rBV6	2663	6113	0.12%	0.013%
30	16.281	2238	2243	2248	rVB7	8684	13581	0.28%	0.028%
31	17.251	2401	2408	2417	rBV	1465860	2065644	41.86%	4.318%
32	17.351	2418	2425	2442	rVV2	3063683	4420622	89.59%	9.240%
33	17.928	2521	2523	2528	rVB6	5005	7285	0.15%	0.015%
34	18.157	2558	2562	2572	rBV2	28682	44797	0.91%	0.094%
35	19.216	2737	2742	2746	rBV4	35100	50465	1.02%	0.105%
36	19.286	2749	2754	2759	rBV2	31531	47059	0.95%	0.098%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029950.D
Acq On : 23 Feb 2024 09:41
Operator : MA/JU
Sample : P1455-10
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AE3

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Title : SVOA CALIBRATION

37	19.451	2778	2782	2787	rBV6	14741	22647	0.46%	0.047%
38	19.604	2805	2808	2810	rBV3	11827	12444	0.25%	0.026%
39	19.651	2810	2816	2826	rVV	3622292	4934237	100.00%	10.314%
40	21.457	3117	3123	3133	rBV	1519162	2104411	42.65%	4.399%
41	23.669	3491	3499	3511	rBV	2288751	4686633	94.98%	9.796%
42	23.816	3518	3524	3535	rVB	1008178	2100949	42.58%	4.392%




Sum of corrected areas: 47840980

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029950.D
Acq On : 23 Feb 2024 09:41
Operator : MA/JU
Sample : P1455-10
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AE3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

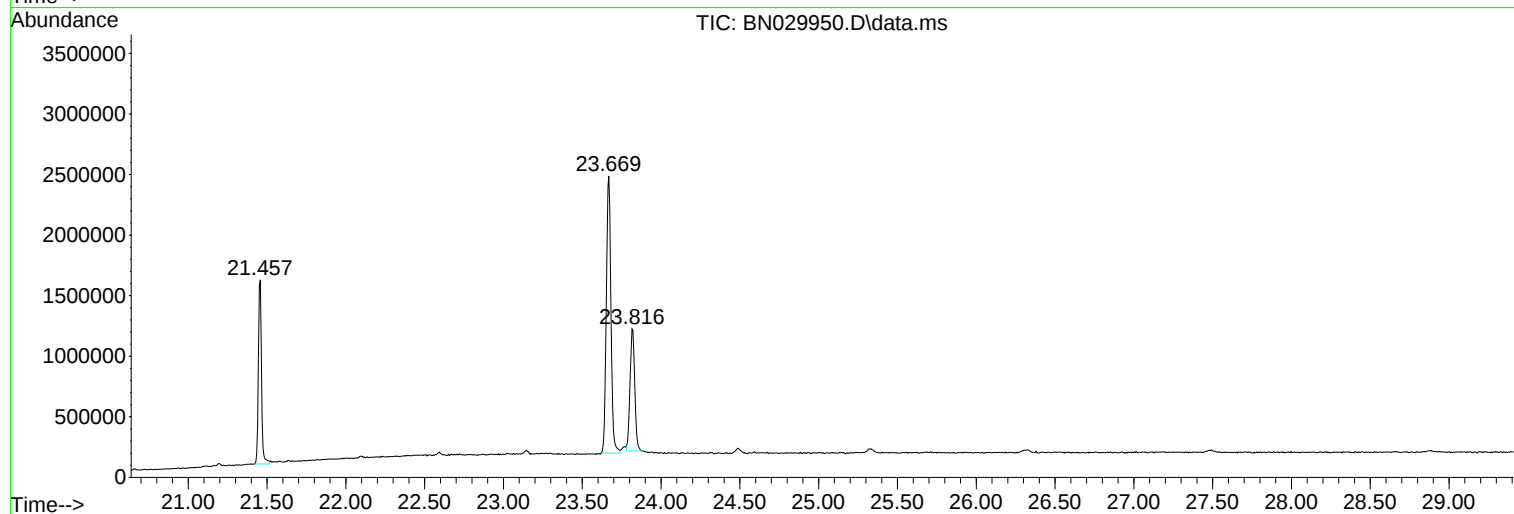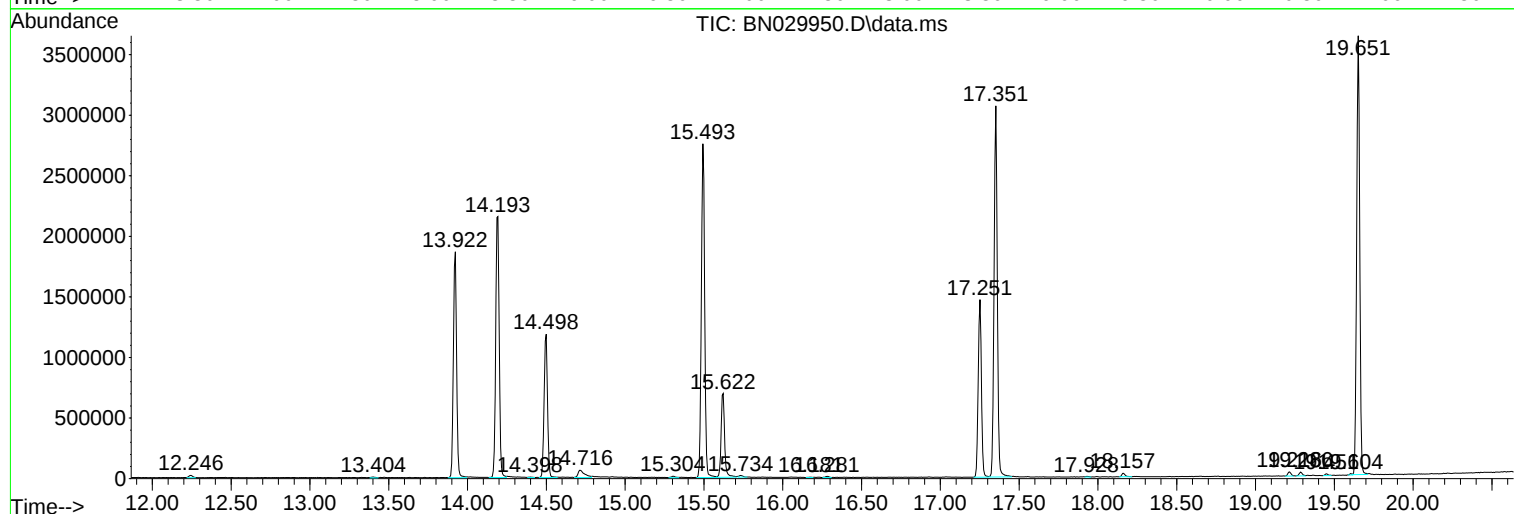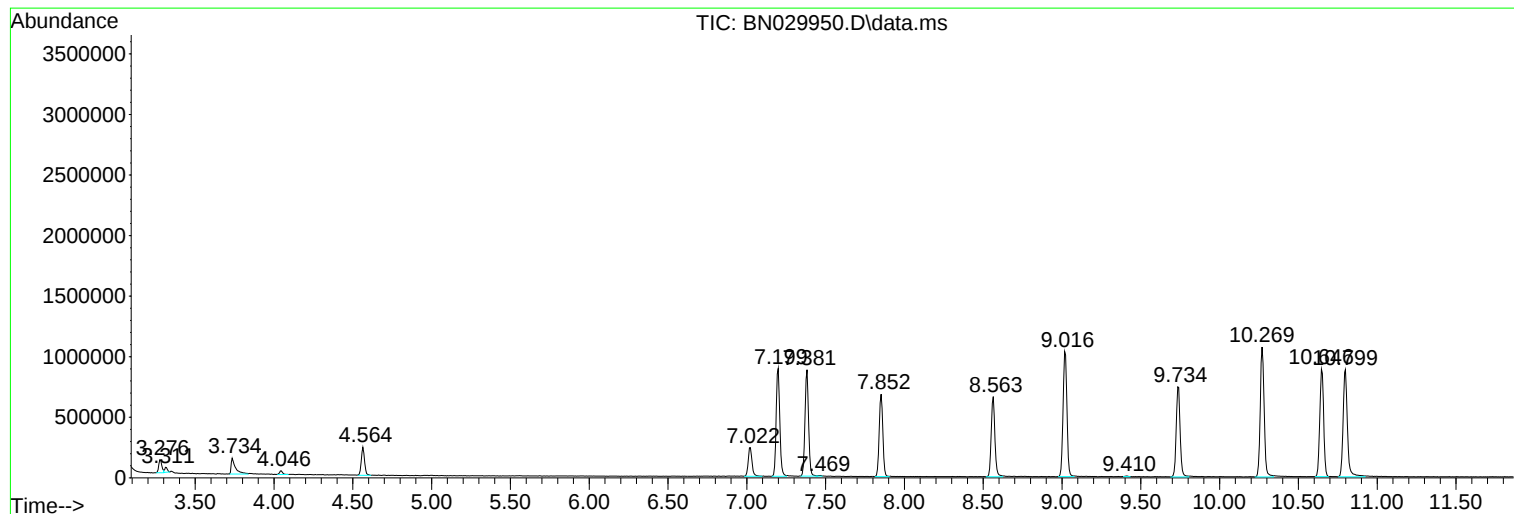

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029950.D
Acq On : 23 Feb 2024 09:41
Operator : MA/JU
Sample : P1455-10
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AE3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029950.D
Acq On : 23 Feb 2024 09:41
Operator : MA/JU
Sample : P1455-10
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AE3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc