

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
 Data File : BN029951.D
 Acq On : 23 Feb 2024 10:26
 Operator : MA/JU
 Sample : P1455-02
 Misc :
 ALS Vial : 73 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AB1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN029951.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.275	26	32	53	rBV	9378897	13906151	100.00%	21.174%
2	3.728	106	109	127	rBV	222661	422763	3.04%	0.644%
3	4.040	158	162	168	rVB	28751	37536	0.27%	0.057%
4	4.558	245	250	260	rVB	469135	686726	4.94%	1.046%
5	7.016	662	668	678	rBV	252424	412870	2.97%	0.629%
6	7.193	689	698	713	rBV	935759	1484893	10.68%	2.261%
7	7.375	721	729	740	rBV	918070	1470861	10.58%	2.240%
8	7.846	803	809	820	rBV	747458	1258398	9.05%	1.916%
9	8.557	923	930	943	rBV	667642	1115976	8.03%	1.699%
10	9.016	1000	1008	1020	rBV	1092821	1805844	12.99%	2.750%
11	9.734	1121	1130	1142	rBV	840359	1385234	9.96%	2.109%
12	10.269	1213	1221	1234	rBV	1145663	1955621	14.06%	2.978%
13	10.646	1277	1285	1298	rBV	1036324	1706173	12.27%	2.598%
14	10.793	1303	1310	1327	rBV	890870	1699533	12.22%	2.588%
15	12.240	1550	1556	1564	rBV2	19686	38129	0.27%	0.058%
16	13.398	1750	1753	1761	rVB7	8696	15220	0.11%	0.023%
17	13.922	1835	1842	1858	rBV	2044017	2863139	20.59%	4.359%
18	14.192	1880	1888	1900	rBV	2362417	3490247	25.10%	5.314%
19	14.498	1933	1940	1951	rBV	1321349	1970974	14.17%	3.001%
20	14.716	1971	1977	1990	rBV2	74821	201697	1.45%	0.307%
21	15.492	2102	2109	2124	rBV	2807090	4251506	30.57%	6.473%
22	15.622	2124	2131	2145	rVV	829088	1204692	8.66%	1.834%
23	15.733	2147	2150	2156	rVB3	14128	21900	0.16%	0.033%
24	17.251	2401	2408	2418	rBV	1652047	2325341	16.72%	3.541%
25	17.351	2418	2425	2444	rVB2	3174023	4546445	32.69%	6.922%
26	18.163	2558	2563	2569	rBV2	64958	95187	0.68%	0.145%
27	19.216	2737	2742	2749	rBV2	38921	59250	0.43%	0.090%
28	19.286	2749	2754	2757	rBV	35008	54585	0.39%	0.083%
29	19.451	2778	2782	2787	rBV5	43060	59371	0.43%	0.090%
30	19.604	2805	2808	2810	rBV3	22778	26660	0.19%	0.041%
31	19.651	2810	2816	2826	rVV	3699884	5203073	37.42%	7.922%
32	20.657	2985	2987	2993	rBV6	13713	18071	0.13%	0.028%
33	21.192	3076	3078	3084	rVB7	24941	32956	0.24%	0.050%
34	21.457	3117	3123	3138	rBV	1776305	2413330	17.35%	3.675%
35	23.668	3491	3499	3510	rBV2	2419613	4944952	35.56%	7.529%
36	23.821	3518	3525	3538	rVB2	1169454	2491442	17.92%	3.793%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029951.D
Acq On : 23 Feb 2024 10:26
Operator : MA/JU
Sample : P1455-02
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AB1

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 65676746

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029951.D
Acq On : 23 Feb 2024 10:26
Operator : MA/JU
Sample : P1455-02
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AB1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

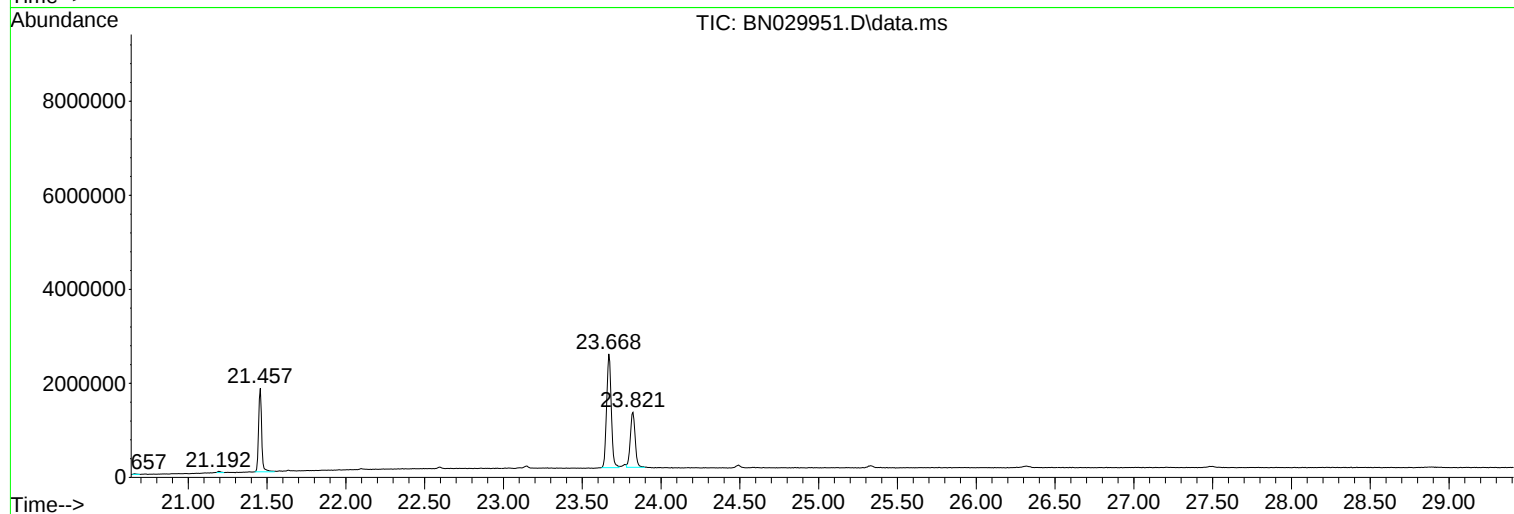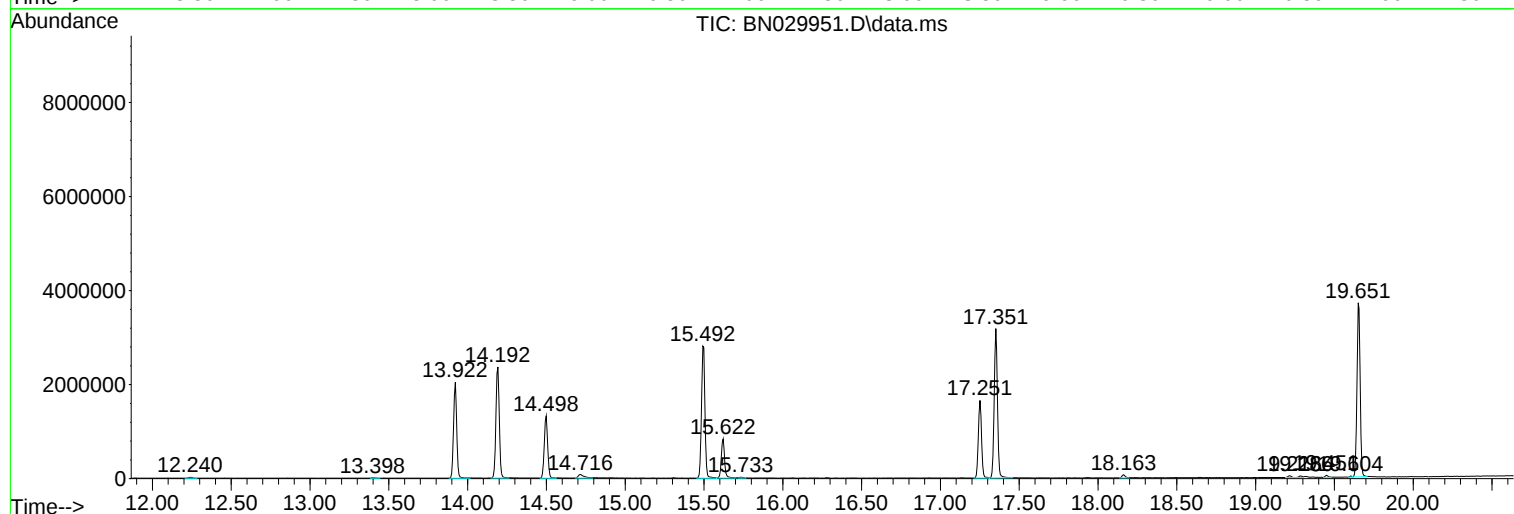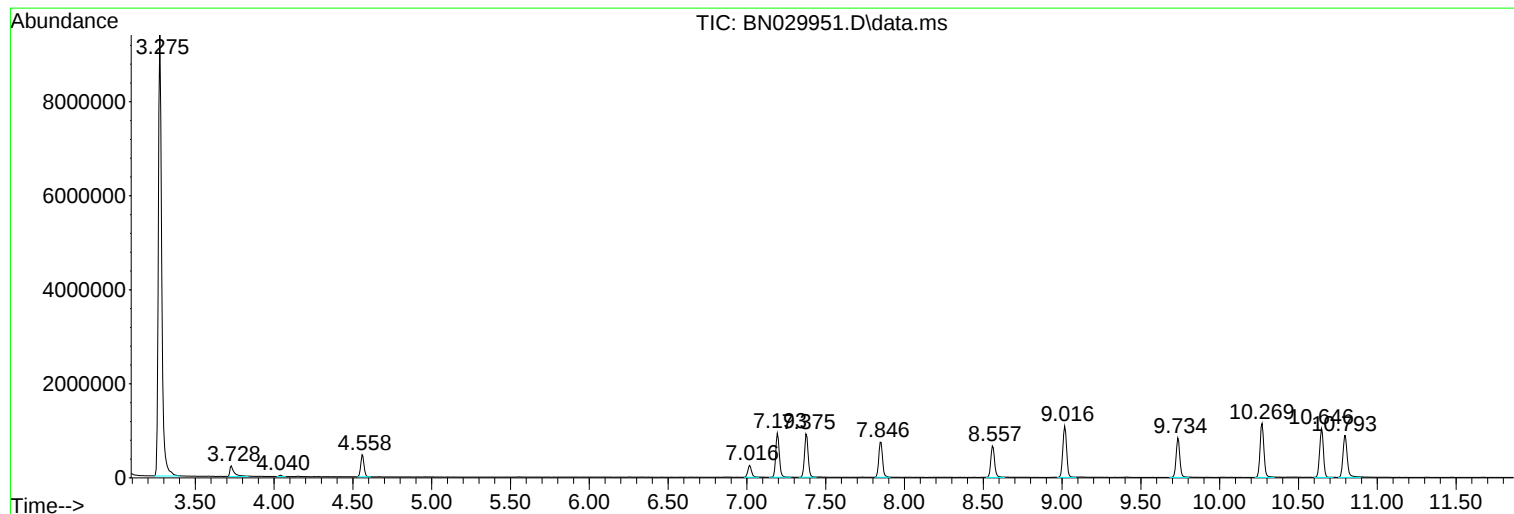

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029951.D
Acq On : 23 Feb 2024 10:26
Operator : MA/JU
Sample : P1455-02
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AB1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022124\
Data File : BN029951.D
Acq On : 23 Feb 2024 10:26
Operator : MA/JU
Sample : P1455-02
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AB1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN020724.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc