

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN022219\
 Data File : BN004474.D
 Acq On : 22 Feb 2019 11:02
 Operator : JU/SJ
 Sample : K1491-17
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB5A3

Quant Time: Feb 22 16:59:02 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 21 22:12:25 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.74	152	21398	20.00	ng/ul	0.00
18) Naphthalene-d8	10.53	136	105388	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.38	164	79724	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.13	188	218814	20.00	ng/ul	0.00
78) Chrysene-d12	21.33	240	301193	20.00	ng/ul	0.00
86) Perylene-d12	23.60	264	364414	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	0.00	96	0	0.00	ng/uL
5) Phenol-d5	0.00	99	0	0.00	ng/ul
7) Bis-(2-Chloroethyl)ether-d	0.00	67	0d	0.00	ng/ul
9) 2-Chlorophenol-d4	0.00	132	0	0.00	ng/ul
13) 4-Methylphenol-d8	0.00	113	0	0.00	ng/ul
19) Nitrobenzene-d5	0.00	128	0	0.00	ng/ul
22) 2-Nitrophenol-d4	0.00	143	0	0.00	ng/ul
26) 2,4-Dichlorophenol-d3	0.00	165	0	0.00	ng/ul
29) 4-Chloroaniline-d4	0.00	131	0	0.00	ng/ul
44) Dimethylphthalate-d6	0.00	166	0	0.00	ng/ul
47) Acenaphthylene-d8	0.00	160	0	0.00	ng/ul
52) 4-Nitrophenol-d4	0.00	143	0	0.00	ng/ul
58) Fluorene-d10	0.00	176	0	0.00	ng/ul
63) 4,6-Dinitro-2-methylphenol	0.00	200	0	0.00	ng/ul
71) Anthracene-d10	0.00	188	0d	0.00	ng/ul
79) Pyrene-d10	0.00	212	0	0.00	ng/ul
90) Benzo(a)pyrene-d12	0.00	264	0d	0.00	ng/ul


Target Compounds				Qvalue
84) Bis(2-ethylhexyl)phthalate	21.23	149	8829	1.029 ng/ul 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN022219\
Data File : BN004474.D
Acq On : 22 Feb 2019 11:02
Operator : JU/SJ
Sample : K1491-17
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CB5A3

Quant Time: Feb 22 16:59:02 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 21 22:12:25 2019
Response via : Initial Calibration

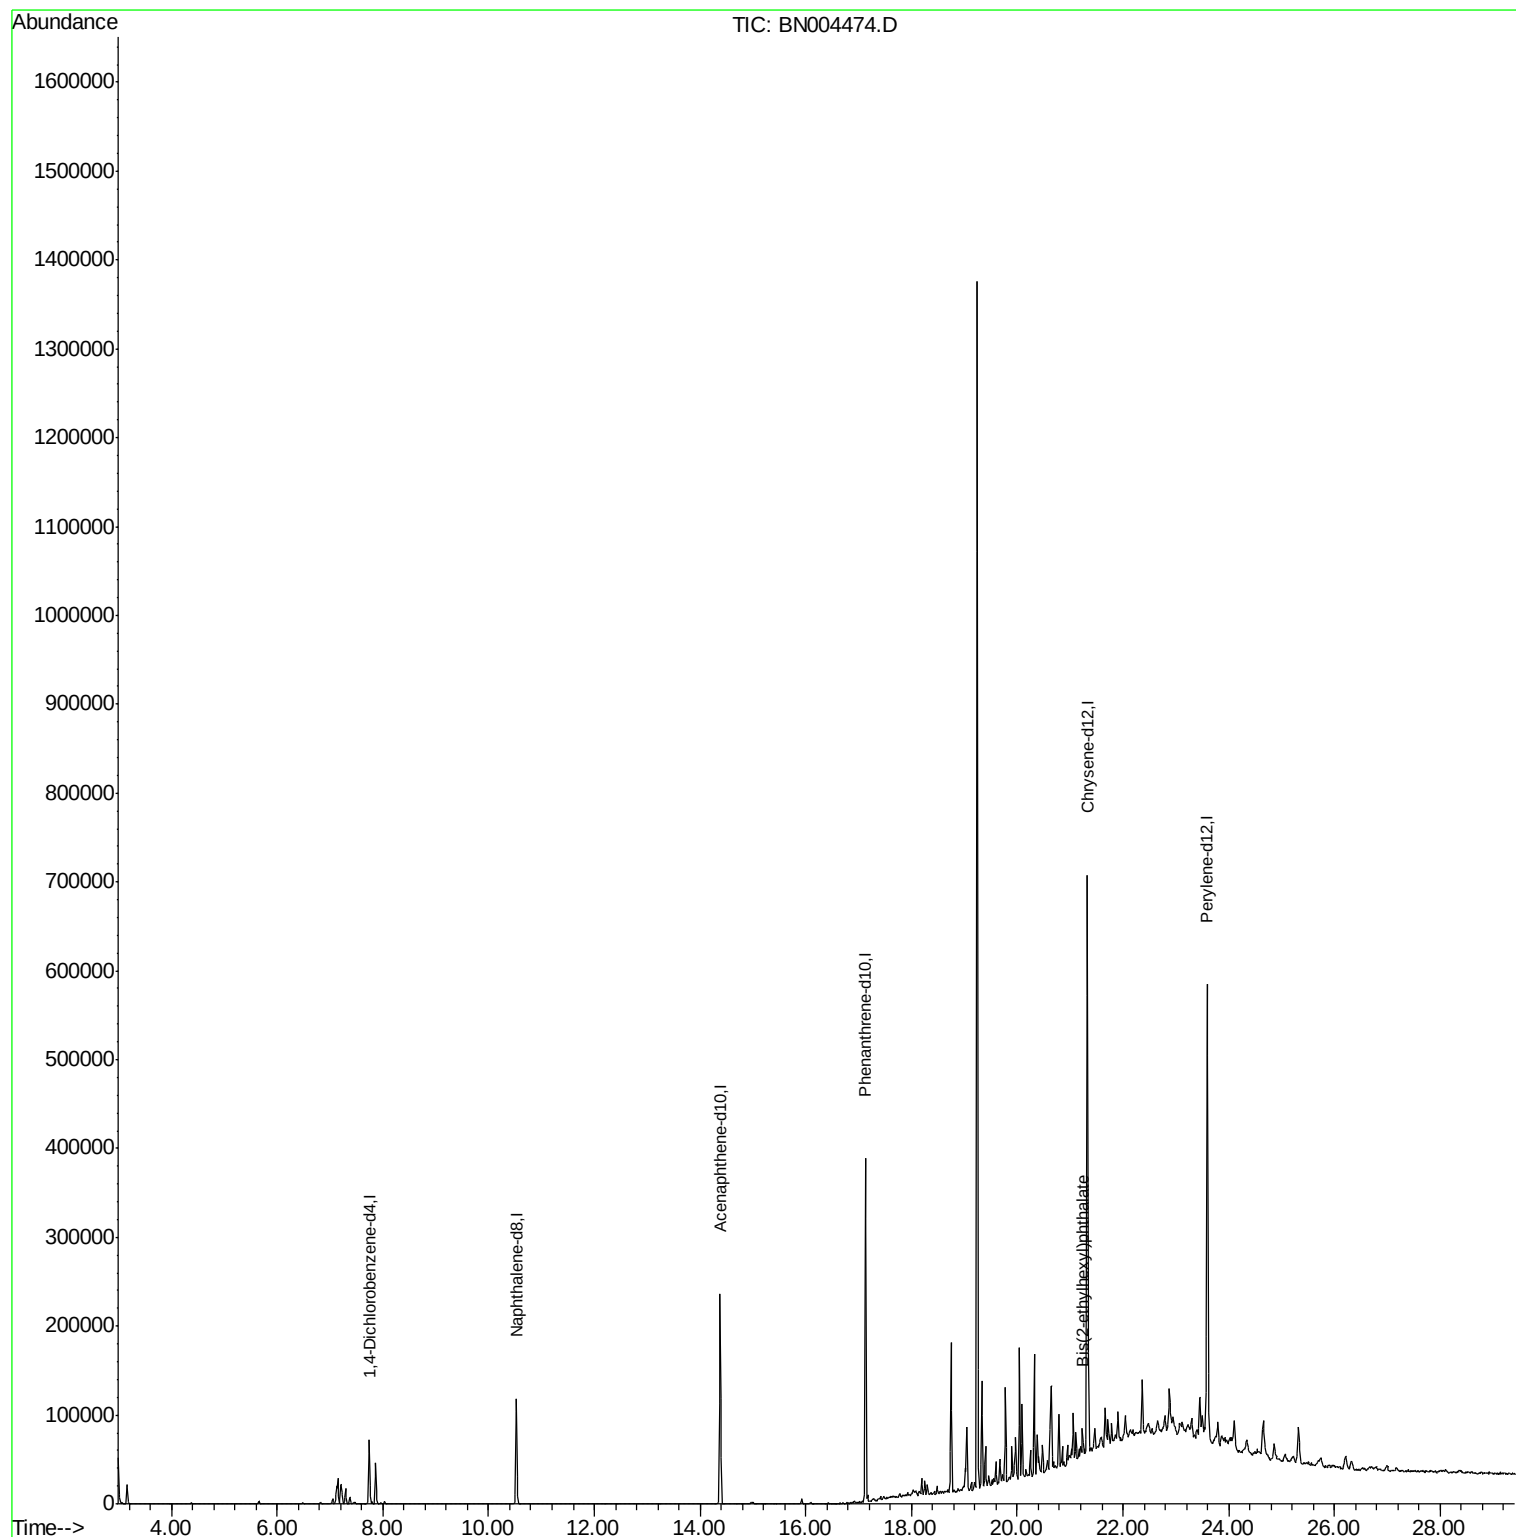

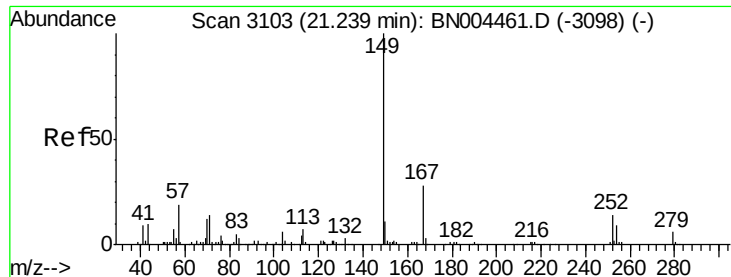

#84

Bis(2-ethylhexyl)phthalate

Concen: 1.029 ng/ul

RT: 21.23 min Scan# 3102

Delta R.T. -0.01 min

Lab File: BN004474.D

Acq: 22 Feb 2019 11:02

Instrument :

BNA_N

ClientSampleId :

CB5A3


Tgt Ion:149 Resp: 8829

Ion Ratio Lower Upper

149 100

167 29.6 22.7 34.1

279 5.7 4.3 6.5

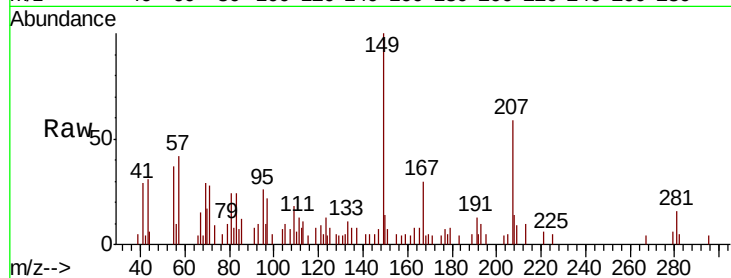

Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

