

m/z	Abundance
39.00	980.0
43.90	352.0
50.00	3590.0
51.00	14162.0
52.00	757.0
56.00	465.0
57.00	1068.0
62.90	617.0
68.20	316.0
69.00	15835.0
74.00	1710.0
75.00	2764.0
76.00	930.0
77.00	17680.0
78.00	1218.0
78.90	1385.0
80.00	968.0
81.00	1274.0
81.90	331.0
83.00	338.0
86.00	485.0
91.00	347.0
92.00	332.0
93.00	2134.0
98.00	1924.0
98.90	1519.0
101.00	795.0
103.90	511.0
105.00	504.0
107.00	5978.0
108.00	885.0
110.00	10949.0
111.00	1801.0
116.00	329.0
117.00	5027.0
118.00	415.0
122.00	382.0
122.90	631.0
123.90	318.0
127.00	21472.0
128.00	1785.0
129.00	8659.0
130.00	795.0
134.90	700.0
136.00	306.0
137.00	490.0
141.00	1074.0
142.00	383.0
142.80	324.0
147.00	585.0
148.00	1293.0
148.90	324.0
152.90	388.0
155.00	648.0
156.00	916.0
159.90	342.0
161.00	564.0
165.00	380.0
165.90	342.0
167.00	2113.0
168.00	1519.0
174.00	497.0
175.00	896.0
176.90	455.0
179.00	1799.0
180.00	1184.0
181.00	575.0
185.10	828.0
186.00	6488.0
187.00	1787.0
189.00	429.0
192.00	472.0
193.00	620.0
196.00	1380.0
198.00	45792.0
199.00	3337.0
203.00	337.0
204.00	1688.0
205.00	2875.0
206.00	12375.0
207.10	1985.0
208.00	461.0
210.90	517.0
216.00	304.0
217.00	3078.0
217.90	456.0
221.00	1885.0
221.80	511.0
223.00	786.0
224.00	6659.0
225.00	1574.0

Instrument :
BNA_N
ClientSampleId :
DFTPP07

227.00	2603.0
228.00	399.0
229.00	532.0
242.00	372.0
243.10	402.0
244.00	5282.0
245.10	727.0
246.00	987.0
255.00	27280.0
256.00	4150.0
257.00	321.0
258.00	1554.0
259.00	302.0
265.00	614.0
272.90	728.0
274.00	2241.0
275.00	12504.0
276.00	1771.0
276.90	1068.0
296.00	3322.0
297.00	473.0
303.00	447.0
315.00	376.0
323.00	1036.0
334.00	762.0
352.00	344.0
354.00	414.0
365.00	1403.0
372.00	595.0
423.00	1828.0
424.00	542.0
441.10	4287.0
442.00	27008.0
443.00	5519.0
444.00	579.0

Instrument :
BNA_N
ClientSampleId :
DFTPP07

m/z	Abundance
39.00	1483.0
43.90	309.0
50.00	5197.0
51.00	20400.0
52.00	1065.0
56.00	584.0
57.00	1530.0
62.00	349.0
63.00	887.0
65.00	484.0
68.20	508.0
69.00	23176.0
74.00	2537.0
75.00	3862.0
76.00	1264.0
77.00	26688.0
78.00	1850.0
79.00	1909.0
80.00	1474.0
81.00	2005.0
81.90	492.0
83.00	488.0
84.90	455.0
86.00	607.0
91.00	576.0
92.00	551.0
93.00	3325.0
98.00	2678.0
99.00	2221.0
101.00	1043.0
102.90	421.0
103.90	760.0
104.90	731.0
107.00	9246.0
108.00	1394.0
110.00	17064.0
111.00	2625.0
112.00	335.0
116.00	596.0
117.00	7867.0
117.90	656.0
122.00	693.0
123.00	990.0
123.90	458.0
125.00	438.0
127.00	34744.0
128.00	2683.0
129.00	13484.0
130.00	1193.0
134.00	402.0
135.00	1193.0
136.00	409.0
136.90	665.0
141.00	1760.0
141.90	617.0
143.00	413.0
146.00	351.0
147.00	1039.0
148.00	2012.0
149.00	494.0
153.00	548.0
154.00	479.0
155.00	894.0
156.00	1510.0
157.00	321.0
157.90	372.0
159.90	665.0
161.00	866.0
164.90	683.0
166.00	539.0
167.00	3472.0
168.00	2055.0
172.10	325.0
173.00	458.0
174.00	799.0
175.00	1451.0
176.10	447.0
176.90	759.0
179.00	2809.0
180.00	2058.0
181.00	766.0
185.00	1372.0
186.00	10893.0
187.00	3322.0
188.00	412.0
189.00	756.0
191.10	374.0
192.00	952.0
193.00	1064.0
196.00	2428.0
198.00	80224.0

Instrument :
BNA_N
ClientSampleId :
DFTPP07

199.00	5696.0
200.00	390.0
201.40	368.0
202.90	531.0
204.00	2899.0
205.00	5026.0
206.00	21560.0
207.00	3361.0
208.00	813.0
209.00	337.0
210.30	407.0
211.00	989.0
216.00	431.0
217.00	5710.0
218.00	776.0
221.00	3513.0
221.90	792.0
223.00	1282.0
224.00	12251.0
225.00	3251.0
226.00	383.0
227.00	5279.0
228.00	693.0
229.00	1053.0
231.00	460.0
233.90	317.0
234.90	383.0
237.00	495.0
242.00	619.0
243.00	735.0
244.00	9736.0
245.00	1342.0
246.00	1934.0
246.90	385.0
249.00	375.0
255.00	51104.0
256.00	7611.0
257.00	595.0
258.00	2867.0
259.00	440.0
265.00	1189.0
273.00	1480.0
274.00	4257.0
275.00	23600.0
276.00	3378.0
277.00	2038.0
277.90	344.0
285.00	392.0
293.00	486.0
296.00	6693.0
297.00	859.0
303.00	829.0
314.00	335.0
315.00	768.0
316.00	354.0
323.00	2287.0
324.00	362.0
326.90	426.0
334.00	1401.0
334.90	407.0
345.90	485.0
352.00	668.0
353.00	478.0
354.00	709.0
365.00	2989.0
366.00	458.0
372.00	1263.0
373.00	310.0
383.00	301.0
402.00	502.0
403.10	605.0
421.00	536.0
422.00	598.0
423.00	3828.0
424.00	1060.0
441.10	10175.0
442.00	63696.0
443.00	12477.0
444.00	1115.0

Instrument :
BNA_N
ClientSampleId :
DFTPP07

m/z	Abundance
39.00	1149.0
44.00	304.0
50.00	4495.0
51.00	17488.0
52.00	945.0
56.00	547.0
57.00	1225.0
63.00	781.0
65.00	473.0
69.00	20352.0
74.00	2275.0
75.00	3312.0
76.00	1212.0
77.00	23968.0
78.00	1649.0
79.00	1734.0
80.00	1286.0
81.00	1885.0
82.00	414.0
83.00	439.0
85.00	392.0
85.90	534.0
90.90	422.0
92.00	499.0
93.00	3054.0
98.00	2409.0
99.00	2020.0
101.00	1091.0
103.00	407.0
104.00	718.0
105.00	731.0
107.00	8550.0
108.00	1192.0
109.00	337.0
110.00	15394.0
111.00	2326.0
116.00	555.0
117.00	7452.0
117.90	472.0
121.90	502.0
123.00	951.0
124.00	488.0
124.90	448.0
127.00	31568.0
128.00	2560.0
129.00	12767.0
130.00	1007.0
134.00	466.0
135.00	1077.0
136.00	461.0
137.00	684.0
141.00	1659.0
142.00	503.0
142.90	398.0
145.90	353.0
147.00	843.0
148.00	1867.0
149.00	442.0
152.90	552.0
154.00	439.0
155.00	996.0
156.00	1558.0
157.00	309.0
157.90	305.0
159.90	548.0
161.00	890.0
165.00	636.0
166.00	481.0
167.00	3421.0
168.00	1787.0
171.90	308.0
173.00	467.0
174.00	814.0
175.00	1503.0
175.90	427.0
177.00	713.0
179.00	2764.0
180.00	2035.0
181.00	922.0
184.00	306.0
185.00	1371.0
186.00	10622.0
187.00	3234.0
188.00	369.0
189.00	715.0
191.00	368.0
192.00	966.0
193.00	1042.0
196.00	2229.0
198.00	78256.0
199.00	5323.0

Instrument :
BNA_N
ClientSampleId :
DFTPP07

200.00	413.0
201.50	382.0
202.90	568.0
204.00	2828.0
205.00	5145.0
206.00	21488.0
207.10	3095.0
208.00	737.0
210.10	374.0
210.90	813.0
216.10	464.0
217.00	5714.0
218.00	837.0
221.00	3468.0
221.80	782.0
223.00	1266.0
224.00	12679.0
225.00	3115.0
226.00	338.0
227.00	4895.0
228.00	696.0
229.00	1011.0
231.00	526.0
235.00	392.0
237.00	463.0
241.00	324.0
241.90	611.0
243.10	723.0
244.00	9795.0
245.00	1320.0
246.00	1943.0
247.00	358.0
248.90	366.0
255.00	52736.0
256.00	7711.0
257.00	613.0
258.00	3099.0
259.00	523.0
265.00	1194.0
273.00	1763.0
274.00	4301.0
275.00	25328.0
276.00	3393.0
277.00	2220.0
278.00	388.0
285.00	419.0
293.00	474.0
296.00	6867.0
297.00	1007.0
303.00	827.0
314.00	388.0
314.90	829.0
316.00	499.0
323.00	2248.0
324.10	453.0
327.00	442.0
334.00	1631.0
335.00	355.0
346.00	568.0
352.00	661.0
353.00	532.0
354.00	840.0
365.00	3427.0
366.00	520.0
372.00	1368.0
373.00	401.0
382.90	367.0
402.10	645.0
403.00	809.0
404.00	344.0
421.10	678.0
422.00	683.0
423.00	4608.0
424.00	1186.0
441.00	12466.0
442.00	78528.0
443.10	14792.0
444.00	1310.0

Instrument :
BNA_N
ClientSampleId :
DFTPP07

Scan 2470 (17.516 min): BN004470.D
DFTPP07

m/z	Abundance
43.90	338.0
207.00	377.0


Instrument :
BNA_N
ClientSampleId :
DFTPP07

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN022219\
 Data File : BN004470.D
 Acq On : 22 Feb 2019 08:41
 Operator : JU/SJ
 Sample : DFTPP07
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP07

Integration File: LSCINT.P

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020719MA.M
 Title : SVOA CALIBRATION
 Last Update : Thu Feb 21 22:12:25 2019

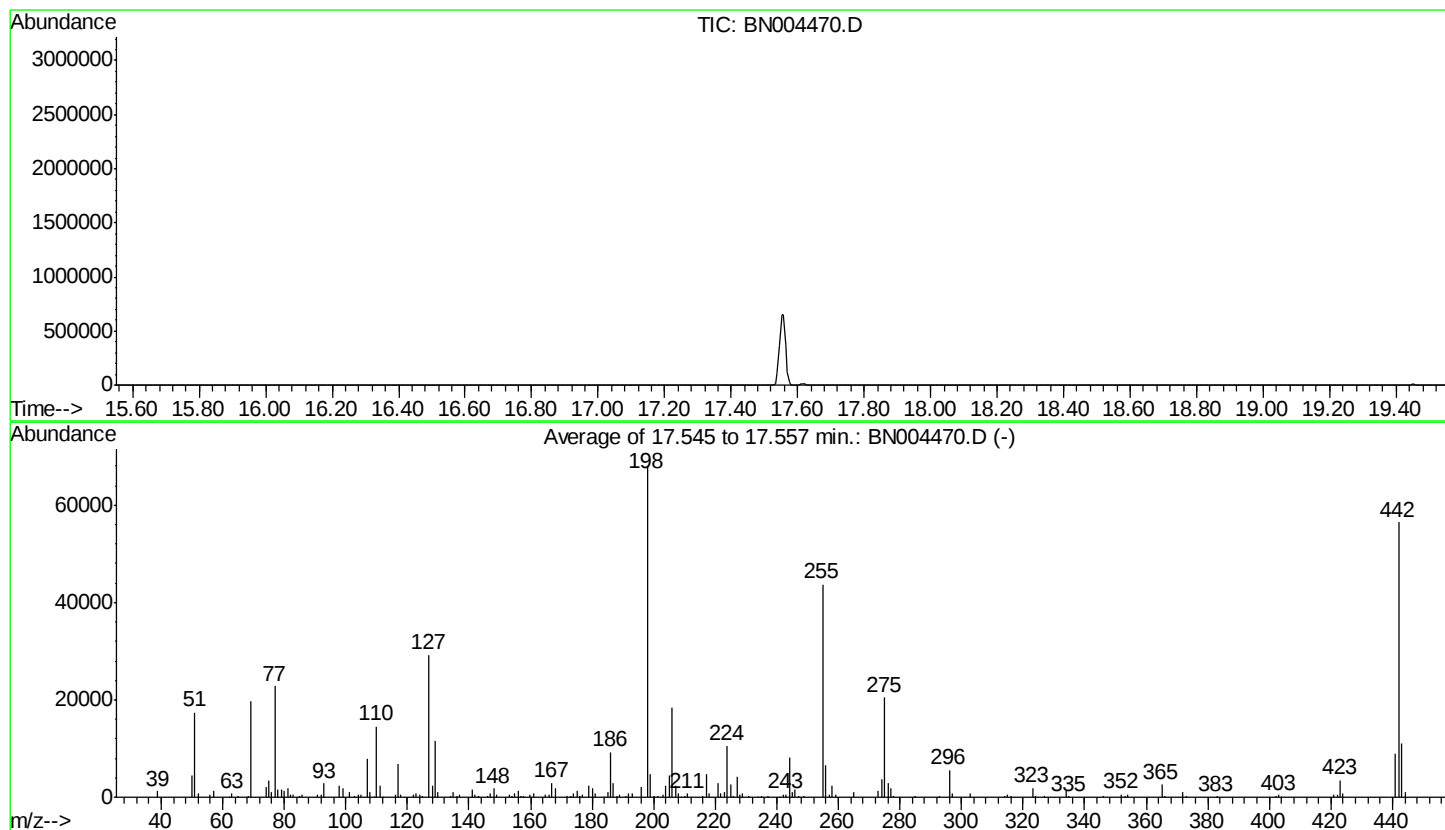

AutoFind: Scans 2475, 2476, 2477; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	25.5	17350	PASS
68	69	0.00	2	1.4	274	PASS
69	198	0.00	100	29.1	19787	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.0	29261	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	68090	PASS
199	198	5	9	7.0	4785	PASS
275	198	10	60	30.1	20477	PASS
365	198	1	100	3.8	2606	PASS
441	198	0.01	100	13.2	8976	PASS
442	198	50	100	82.8	56410	PASS
443	442	15	24	19.4	10929	PASS