
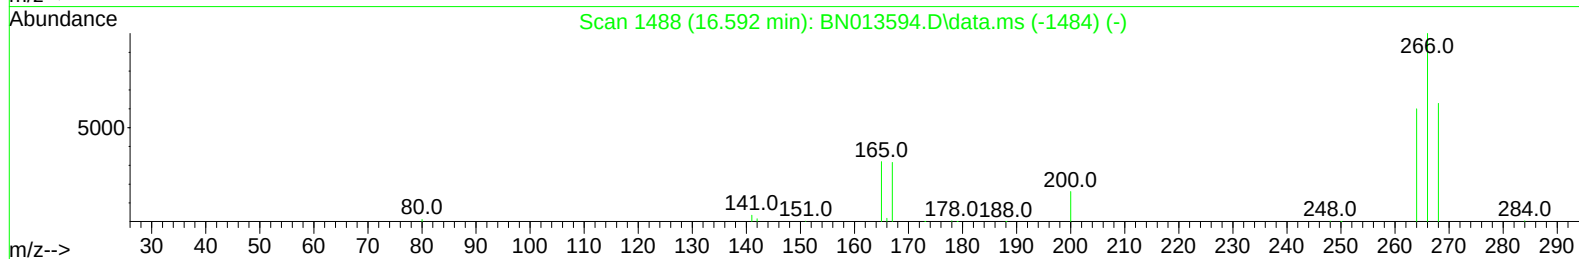
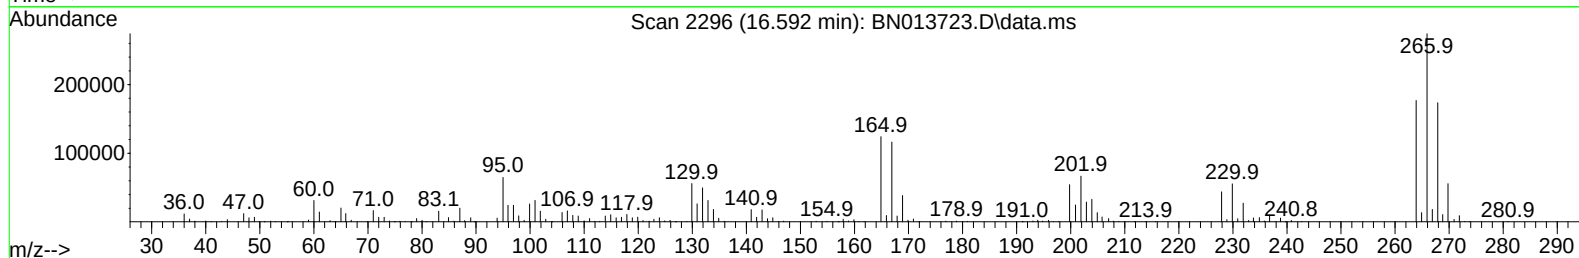


```
Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022221\  
Data File : BN013723.D  
Acq On    : 22 Feb 2021 09:35  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Feb 22 10:10:47 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN020821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 18 10:50:10 2021
Response via : Initial Calibration

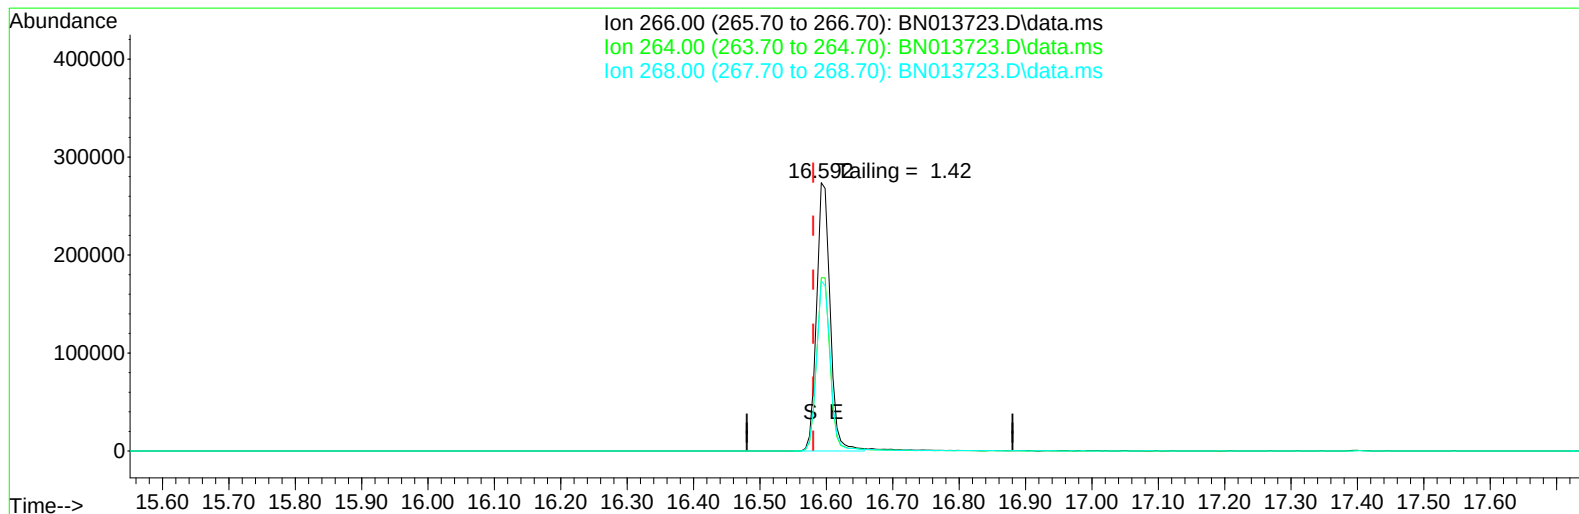

TIC: BN013723.D\data.ms

(24) Pentachlorophenol

16.592min (+ 0.012) 0.00 ng

response **396246**

Ion	Exp%	Act%
266.00	100.00	100.00
264.00	64.50	63.97
268.00	68.30	64.07
0.00	0.00	0.00