
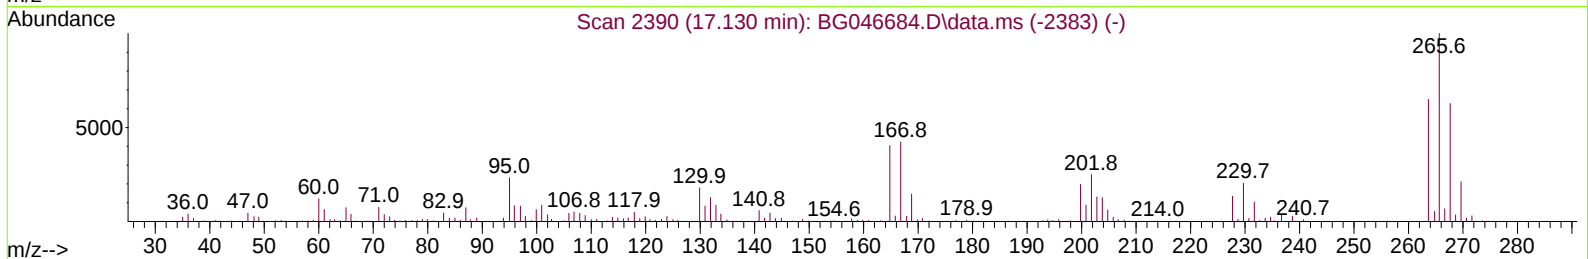
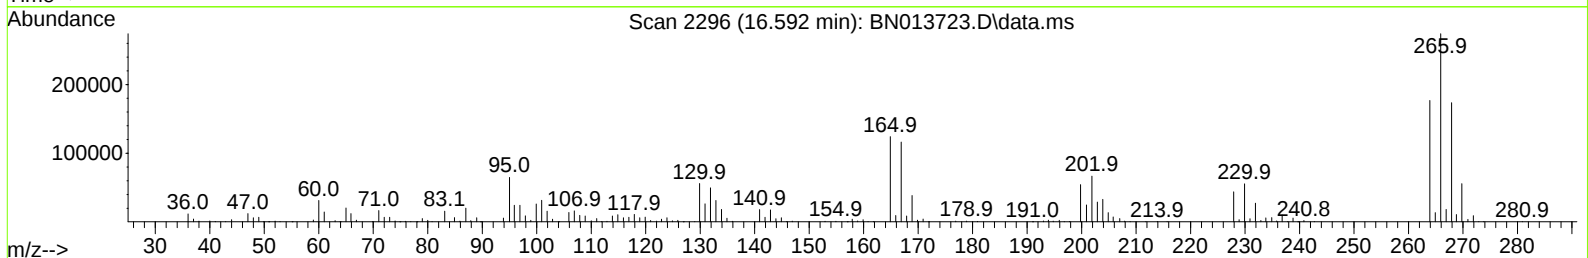


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022221\
 Data File : BN013723.D
 Acq On : 22 Feb 2021 09:35
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 26 04:24:32 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 25 01:54:00 2021
 Response via : Initial Calibration

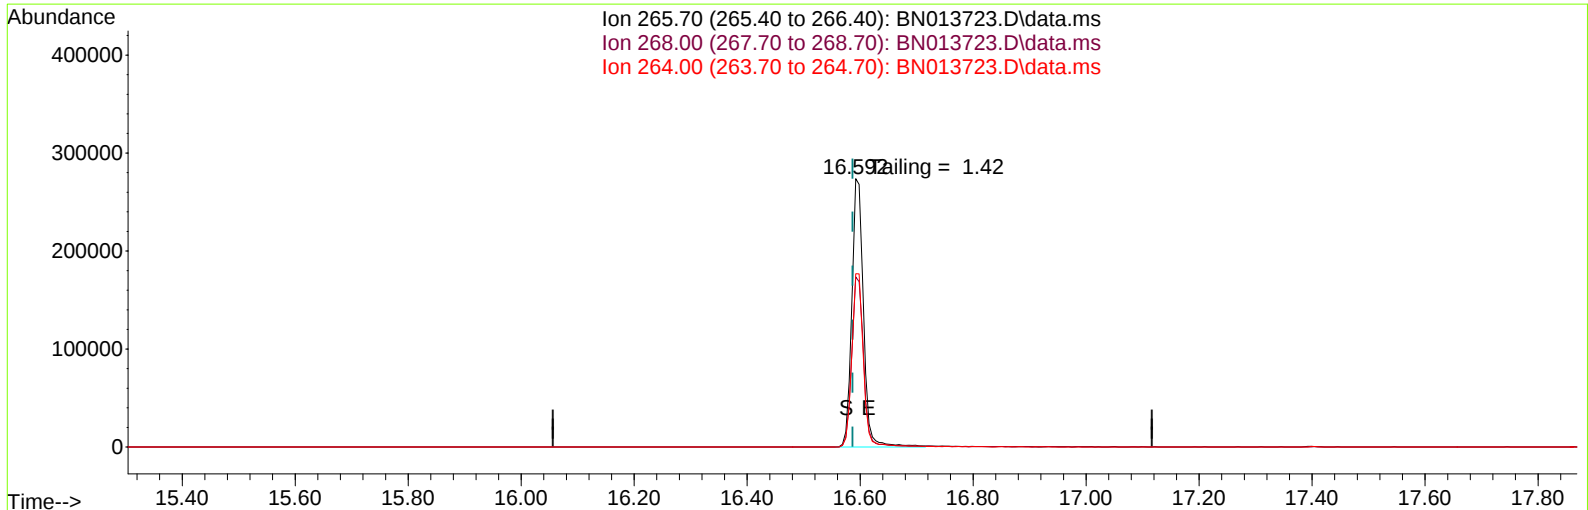

TIC: BN013723.D\data.ms

(70) Pentachlorophenol (C)




16.592min (+ 0.006) 26107.38 ng

response 396246

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.41
264.00	61.60	64.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022221\
Data File : BN013723.D
Acq On : 22 Feb 2021 09:35
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 26 04:24:32 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 25 01:54:00 2021
Response via : Initial Calibration

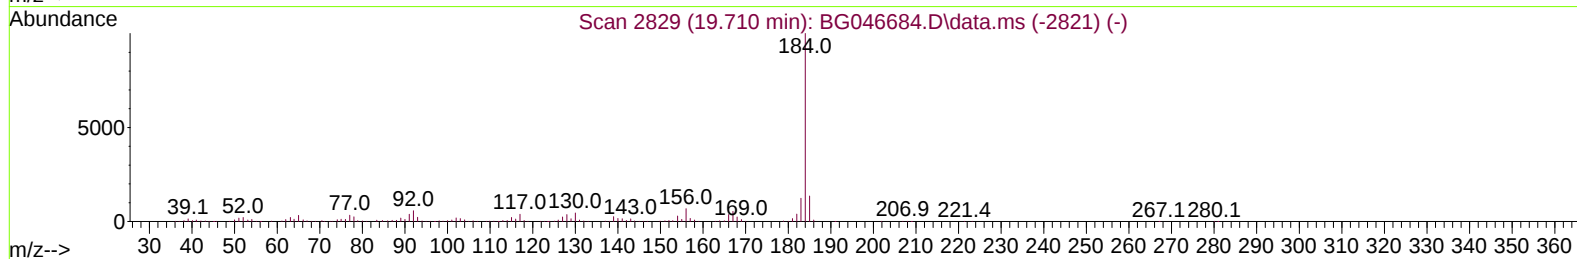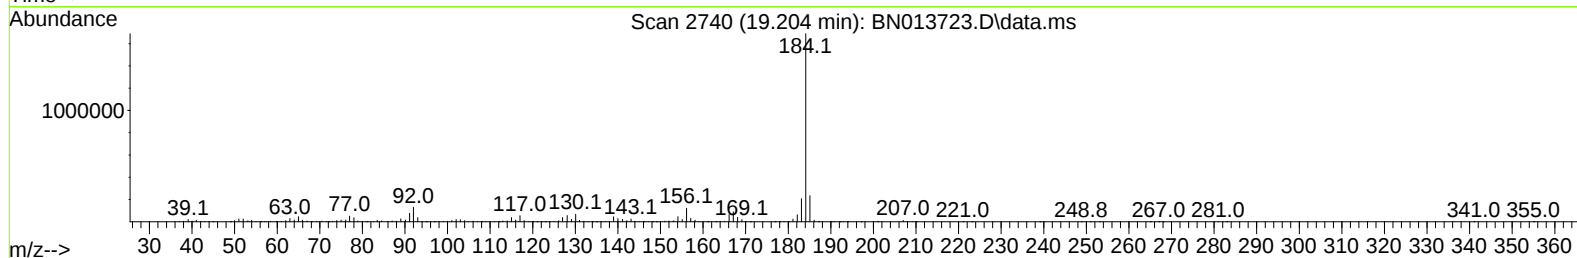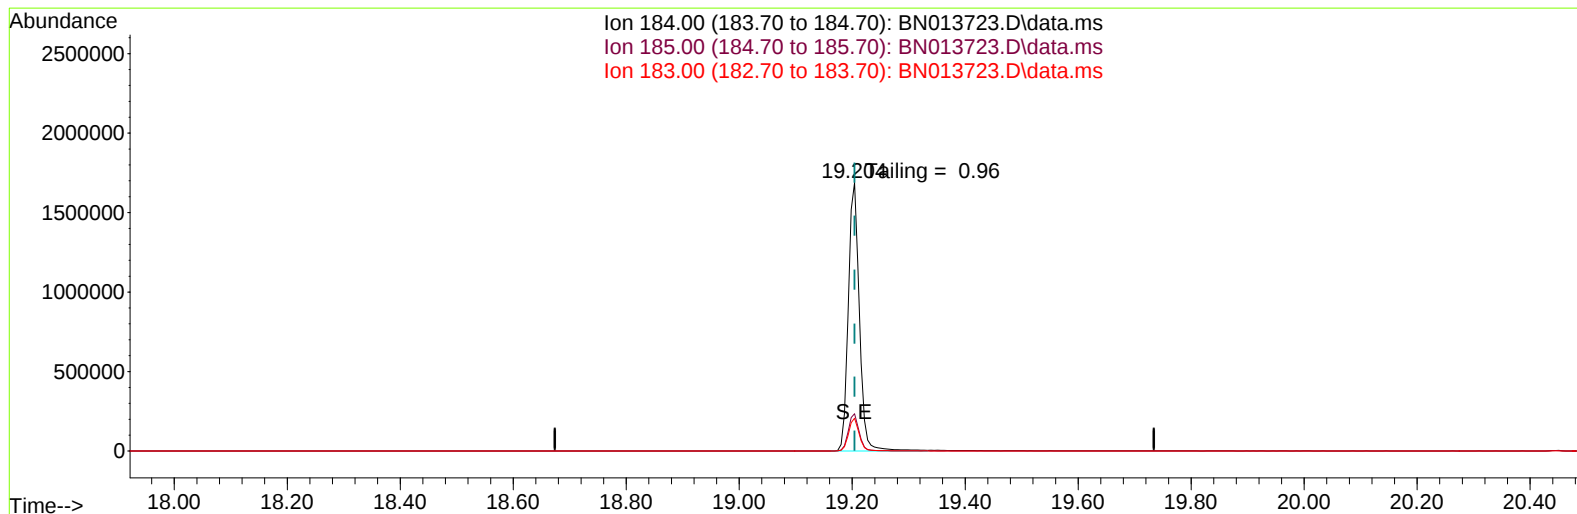

TIC: BN013723.D\data.ms

(77) Benzidine**19.204min (-0.000) 273425.04 ng****response 2300961**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.92
183.00	13.20	12.25
0.00	0.00	0.00