
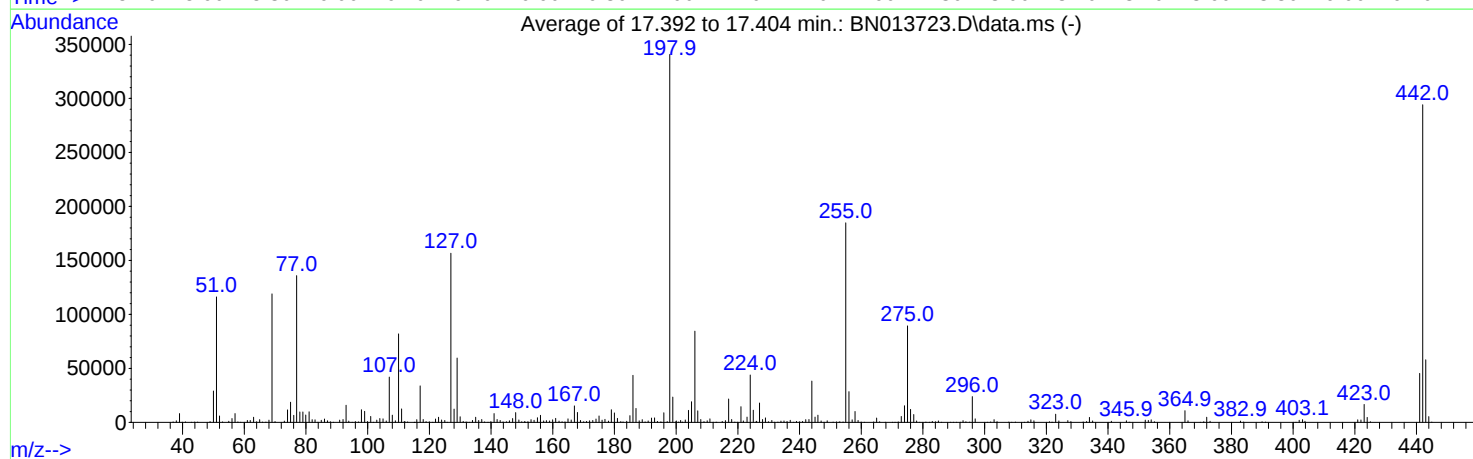


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022221\
 Data File : BN013723.D
 Acq On : 22 Feb 2021 09:35
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN020821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Feb 18 10:50:10 2021

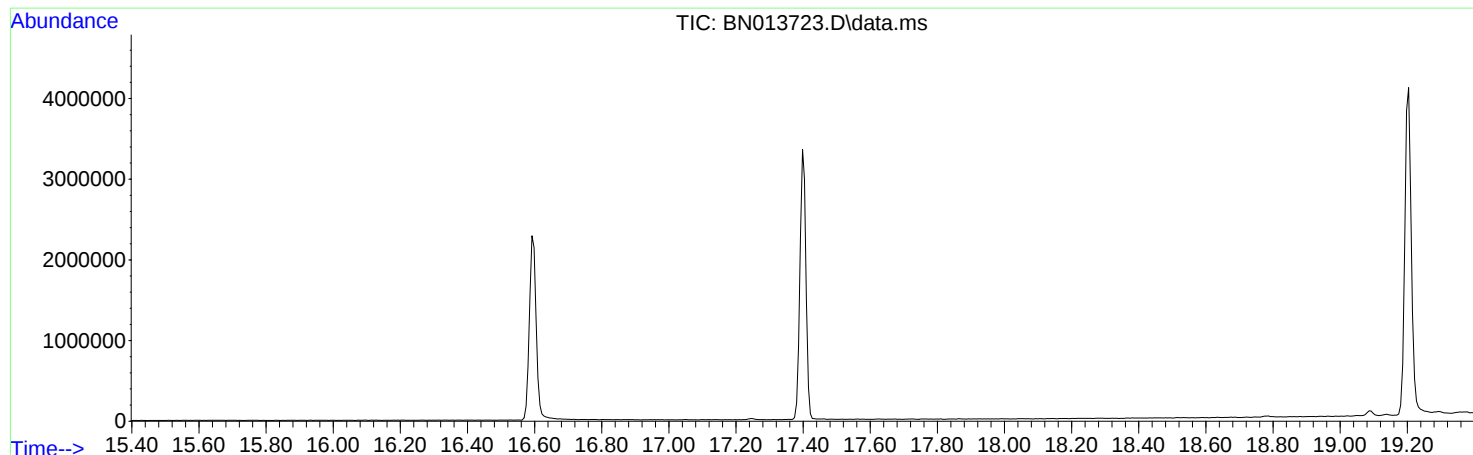

AutoFind: Scans 2432, 2433, 2434; Background Corrected with Scan 2425

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.1	116165	PASS
68	69	0.00	2	1.7	2035	PASS
69	198	0.00	100	34.9	118900	PASS
70	69	0.00	2	0.6	680	PASS
127	198	10	80	46.0	156587	PASS
197	198	0.00	2	0.2	716	PASS
198	198	100	100	100.0	340608	PASS
199	198	5	9	6.9	23419	PASS
275	198	10	60	26.2	89317	PASS
365	198	1	100	3.2	10887	PASS
441	198	0.01	100	13.3	45336	PASS
442	442	50	100	100.0	294144	PASS
443	442	15	24	19.7	57896	PASS

DDT Breakdown




Instrument :
BNA_N
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
02/22/2021	BNA_N	<u>BN013723.D</u>
Compound Name	Response	Retention Time
DDT	1077439	20.44
DDD	116821	20
DDE	12088	19.49
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
128909	1206348	10.69

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022221\
Data File : BN013723.D
Acq On : 22 Feb 2021 09:35
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Feb 26 04:24:32 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 25 01:54:00 2021
Response via : Initial Calibration

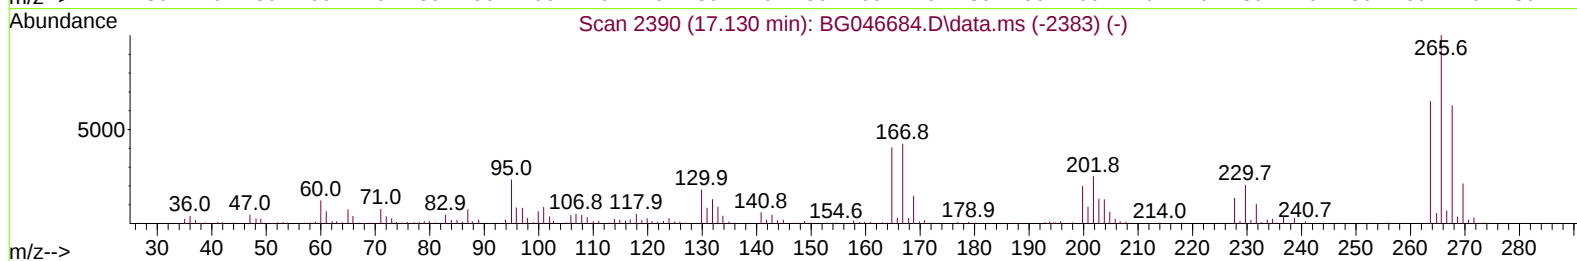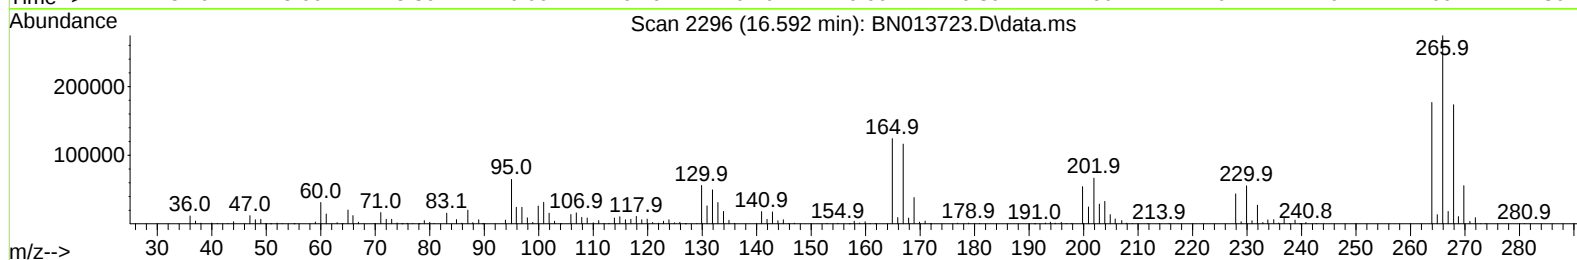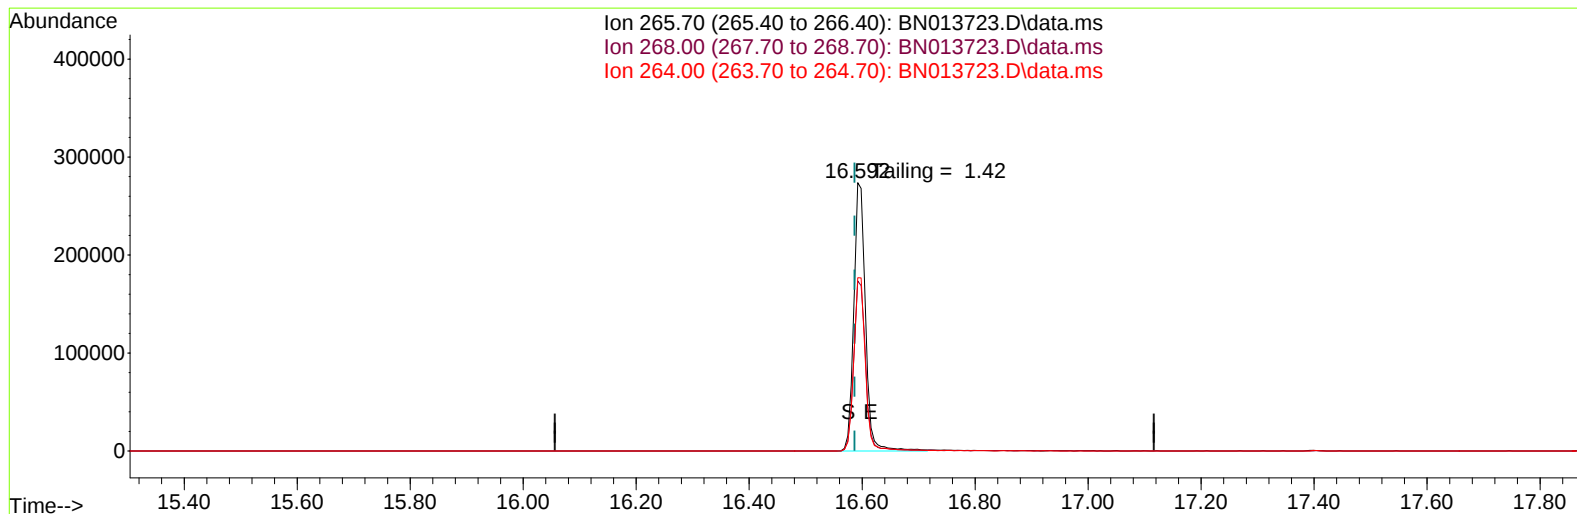

TIC: BN013723.D\data.ms

(70) Pentachlorophenol (C)

16.592min (+ 0.006) 26107.38 ng




response 396246

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.41
264.00	61.60	64.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022221\
 Data File : BN013723.D
 Acq On : 22 Feb 2021 09:35
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Feb 26 04:24:32 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 25 01:54:00 2021
 Response via : Initial Calibration

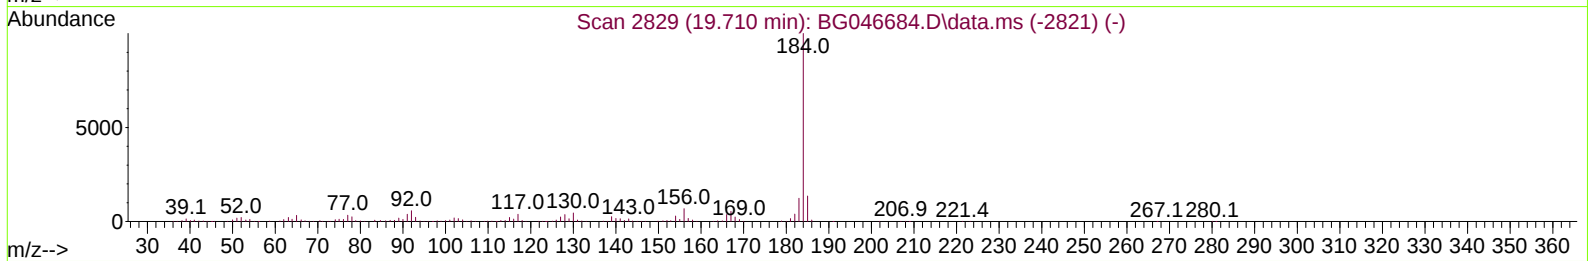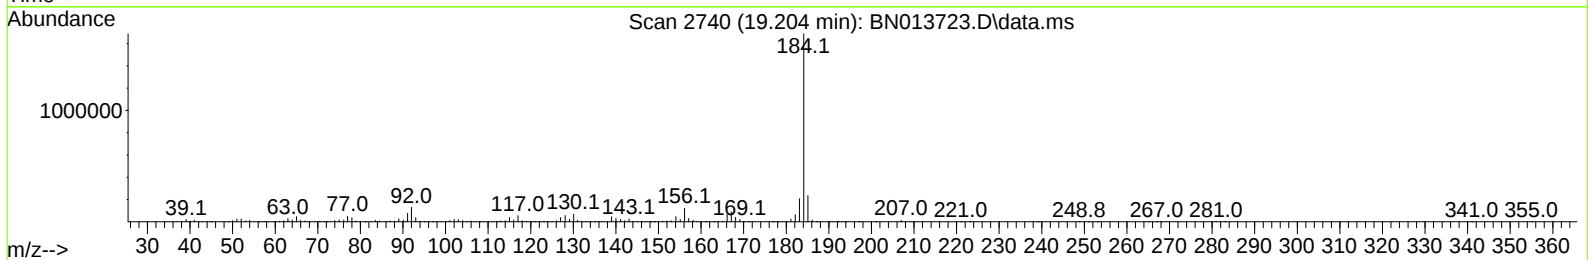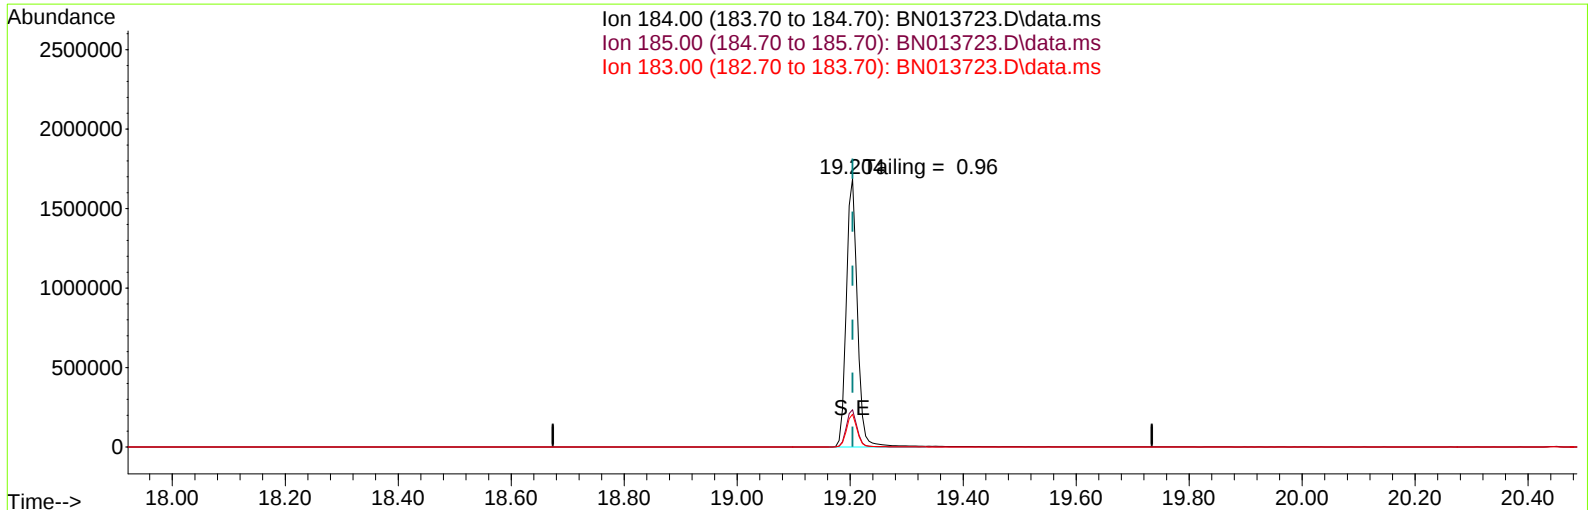

TIC: BN013723.D\data.ms

(77) Benzidine

19.204min (-0.000) 273425.04 ng

response 2300961

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.92
183.00	13.20	12.25
0.00	0.00	0.00