

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022322\
 Data File : BN018703.D
 Acq On : 23 Feb 2022 18:32
 Operator : CG/JU
 Sample : N1587-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 PRPH-1-GW

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 02/24/2022
 Supervised By :mohammad ahmed 02/24/2022

Quant Time: Feb 24 01:37:04 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN022222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 22 16:23:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.919	152	7568	0.400	ng	0.00
7) Naphthalene-d8	10.722	136	19620	0.400	ng	# 0.00
13) Acenaphthene-d10	14.549	164	10200	0.400	ng	0.00
19) Phenanthrene-d10	17.287	188	19763	0.400	ng	0.00
29) Chrysene-d12	21.467	240	13689	0.400	ng	# 0.00
35) Perylene-d12	23.860	264	11183	0.400	ng	# 0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.471	112	2107	0.122	ng	0.00
5) Phenol-d6	7.067	99	1530	0.077	ng	0.00
8) Nitrobenzene-d5	9.067	82	3742m	0.247	ng	0.00
11) 2-Methylnaphthalene-d10	12.310	152	7669	0.259	ng	0.00
14) 2,4,6-Tribromophenol	16.025	330	1086	0.273	ng	0.00
15) 2-Fluorobiphenyl	13.180	172	12662	0.262	ng	0.00
27) Fluoranthene-d10	19.312	212	16497	0.308	ng	0.00
31) Terphenyl-d14	19.906	244	10997	0.370	ng	0.00
Target Compounds						Qvalue
9) Naphthalene	10.776	128	9511	0.168	ng	97
12) 2-Methylnaphthalene	12.382	142	4729	0.125	ng	95
25) Phenanthrene	17.328	178	2049	0.031	ng	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022322\
Data File : BN018703.D
Acq On : 23 Feb 2022 18:32
Operator : CG/JU
Sample : N1587-02
Misc :
ALS Vial : 15 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
PRPH-1-GW

Quant Time: Feb 24 01:37:04 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN022222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 22 16:23:51 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 02/24/2022
Supervised By :mohammad ahmed 02/24/2022

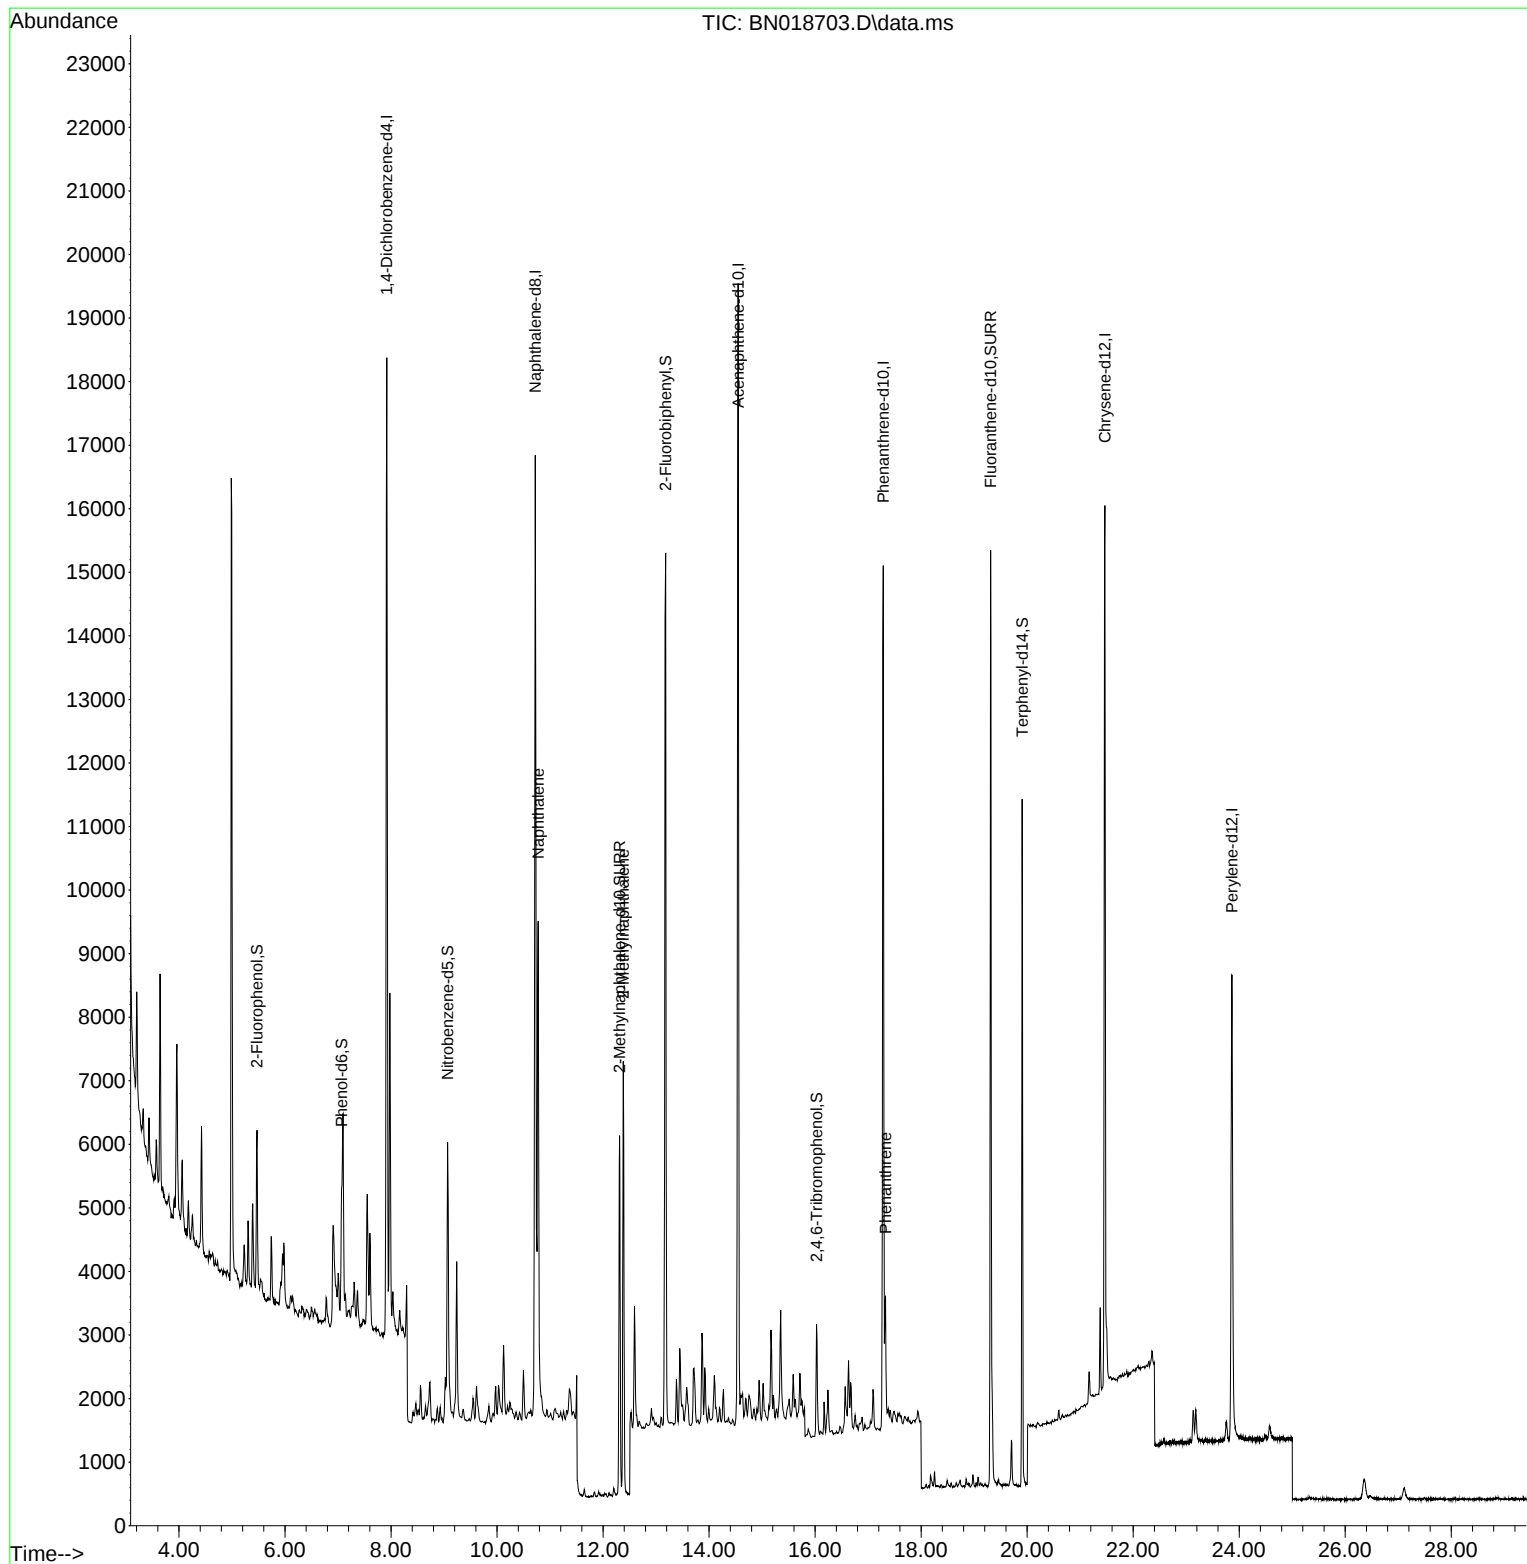

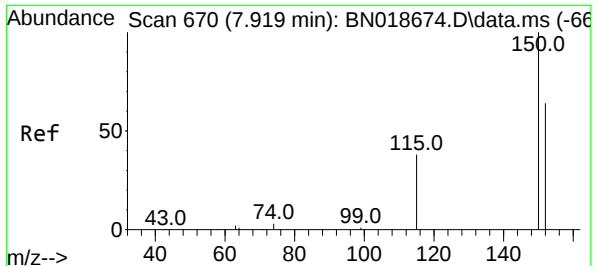

#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.919 min Scan# 61
Delta R.T. 0.000 min
Lab File: BN018703.D
Acq: 23 Feb 2022 18:32




Instrument :
BNA_N
ClientSampleId :
PRPH-1-GW

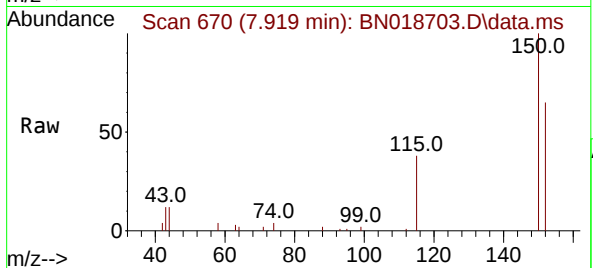

Tgt Ion:152 Resp: 756
Ion Ratio Lower Upper
152 100
150 153.5 121.7 182.5
115 58.9 43.8 65.8




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 02/24/2022
Supervised By :mohammad ahmed 02/24/2022

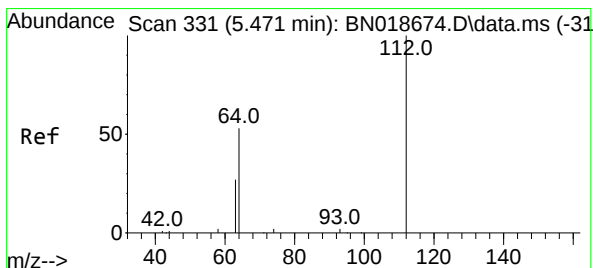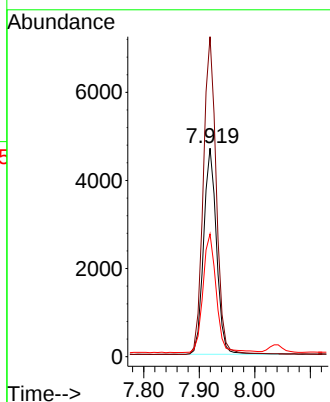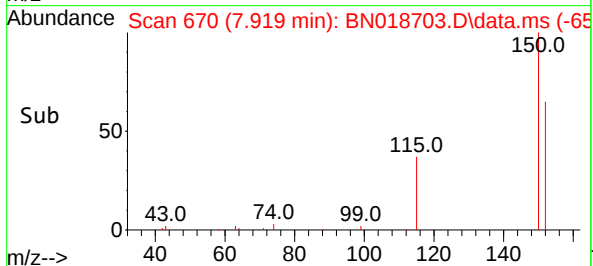

#4
2-Fluorophenol
Concen: 0.122 ng
RT: 5.471 min Scan# 331
Delta R.T. -0.000 min
Lab File: BN018703.D
Acq: 23 Feb 2022 18:32


Tgt Ion:112 Resp: 2107
Ion Ratio Lower Upper
112 100
64 56.8 48.0 72.0
63 29.1 25.3 37.9

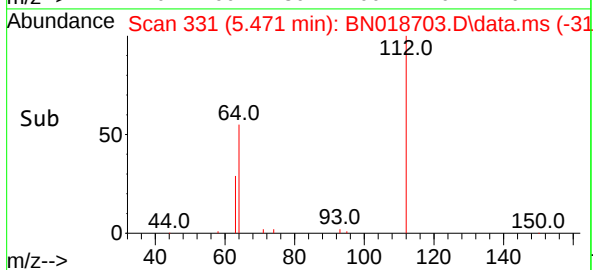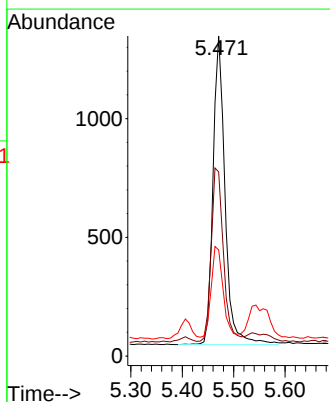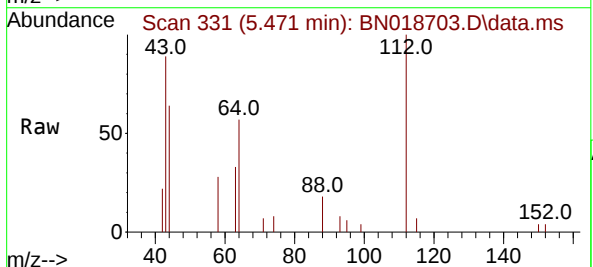

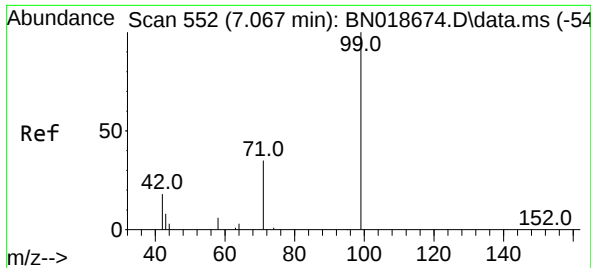

#5
Phenol-d6
Concen: 0.077 ng
RT: 7.067 min Scan# 552
Delta R.T. -0.000 min
Lab File: BN018703.D
Acq: 23 Feb 2022 18:32




Instrument :
BNA_N
ClientSampleId :
PRPH-1-GW

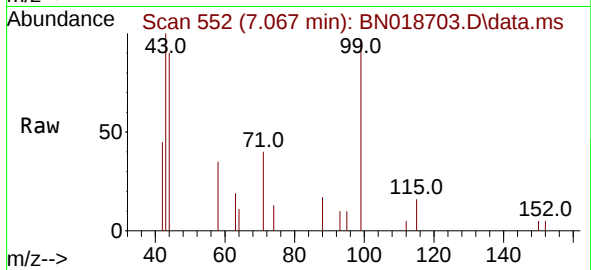


Tgt Ion: 99 Resp: 1530
Ion Ratio Lower Upper
99 100
42 36.0 16.3 24.5
71 43.3 26.8 40.2

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 02/24/2022
Supervised By :mohammad ahmed 02/24/2022

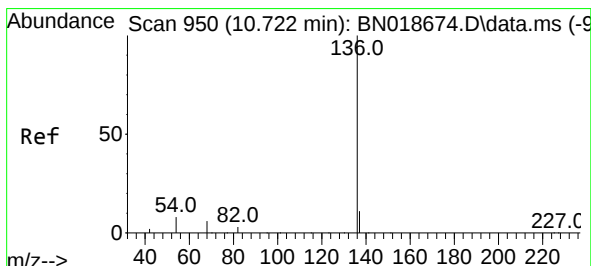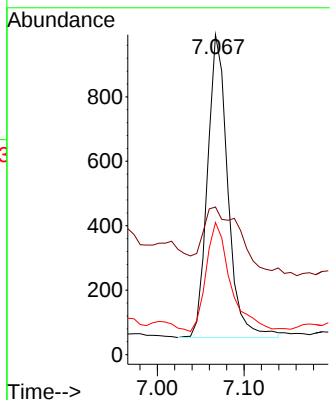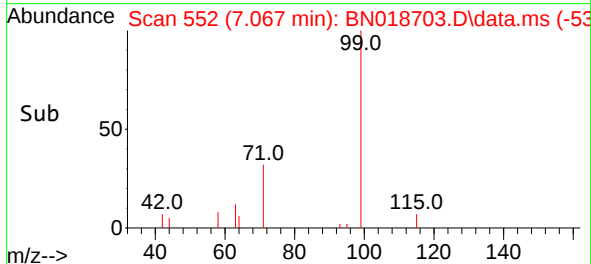


#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.722 min Scan# 950
Delta R.T. -0.000 min
Lab File: BN018703.D
Acq: 23 Feb 2022 18:32

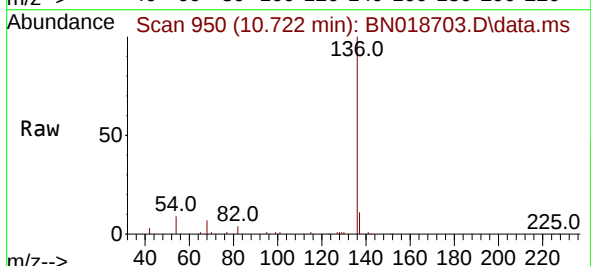

Tgt Ion:136 Resp: 19620
Ion Ratio Lower Upper
136 100
137 11.4 8.8 13.2
54 9.4 5.0 7.6#
68 7.1 4.4 6.6#

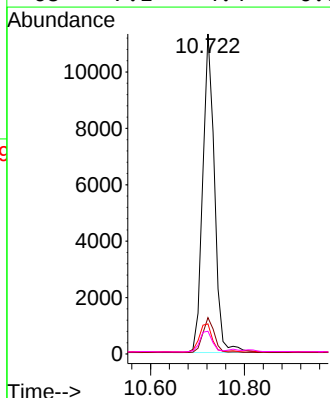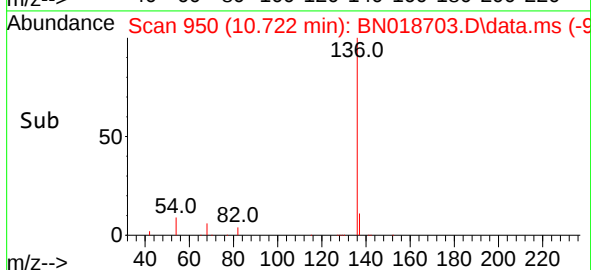

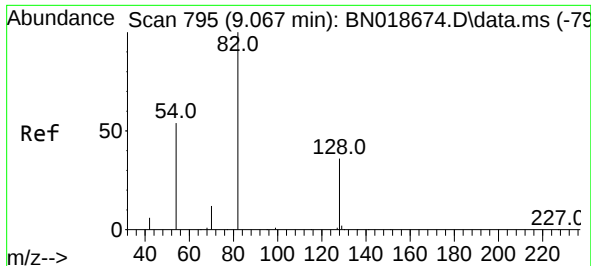

#8
Nitrobenzene-d5
Concen: 0.247 ng m
RT: 9.067 min Scan# 795
Delta R.T. -0.000 min
Lab File: BN018703.D
Acq: 23 Feb 2022 18:32

Instrument :

BNA_N





ClientSampleId :

PRPH-1-GW

Tgt Ion: 82 Resp: 3742
Ion Ratio Lower Upper
82 100
128 36.8 33.7 50.5
54 56.3 36.6 55.0




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 02/24/2022
Supervised By :mohammad ahmed 02/24/2022

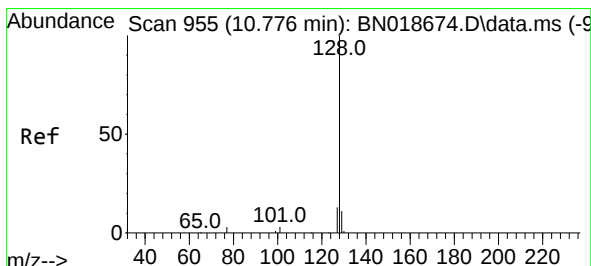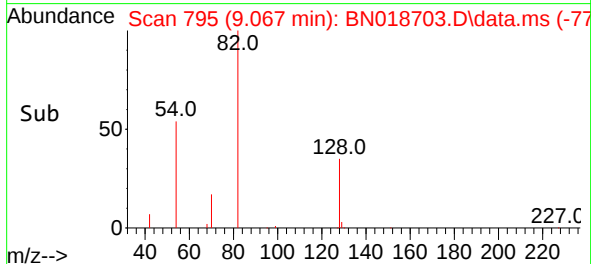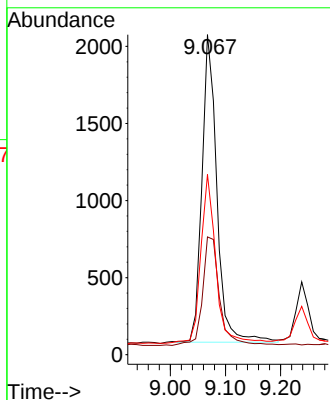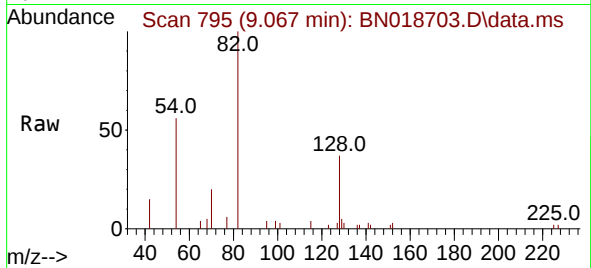

#9
Naphthalene
Concen: 0.168 ng
RT: 10.776 min Scan# 955
Delta R.T. -0.000 min
Lab File: BN018703.D
Acq: 23 Feb 2022 18:32


Tgt Ion:128 Resp: 9511
Ion Ratio Lower Upper
128 100
129 12.4 8.7 13.1
127 13.8 10.4 15.6

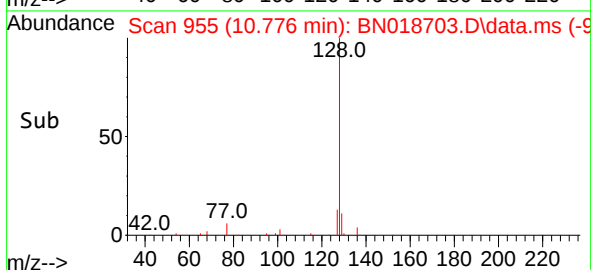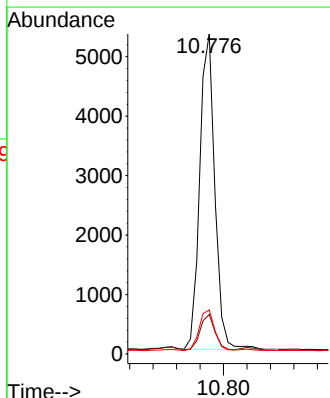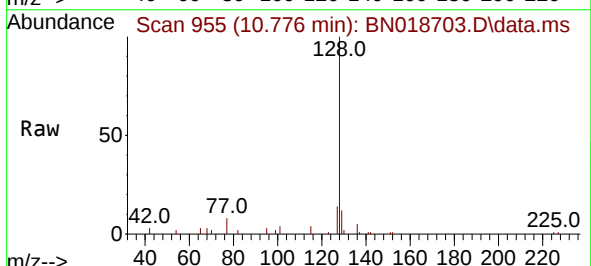

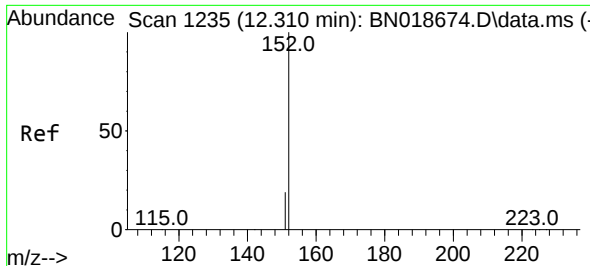

#11
2-Methylnaphthalene-d10
Concen: 0.259 ng
RT: 12.310 min Scan# 1235
Delta R.T. -0.000 min
Lab File: BN018703.D
Acq: 23 Feb 2022 18:32




Instrument :
BNA_N
ClientSampleId :
PRPH-1-GW

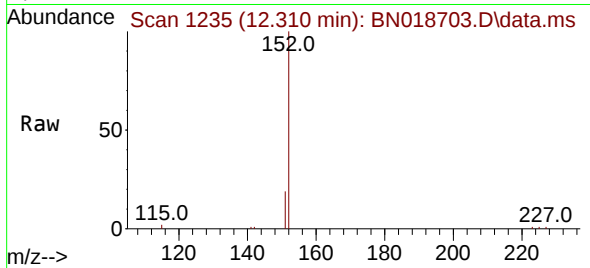


Tgt Ion:152 Resp: 7669
Ion Ratio Lower Upper
152 100
151 20.9 16.2 24.2

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 02/24/2022
Supervised By :mohammad ahmed 02/24/2022

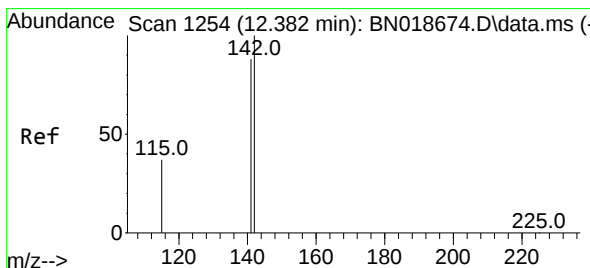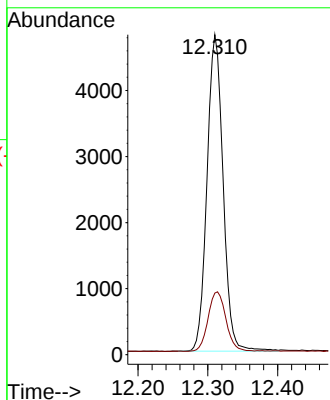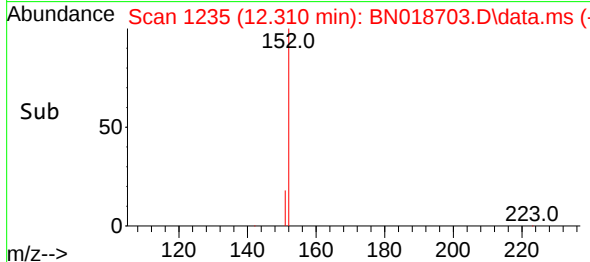


#12
2-Methylnaphthalene
Concen: 0.125 ng
RT: 12.382 min Scan# 1254
Delta R.T. -0.000 min
Lab File: BN018703.D
Acq: 23 Feb 2022 18:32

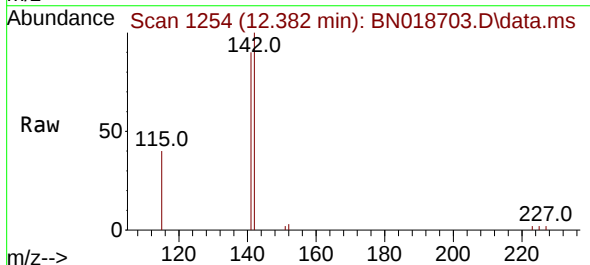


Tgt Ion:142 Resp: 4729
Ion Ratio Lower Upper
142 100
141 90.5 70.0 105.0
115 39.8 27.8 41.8

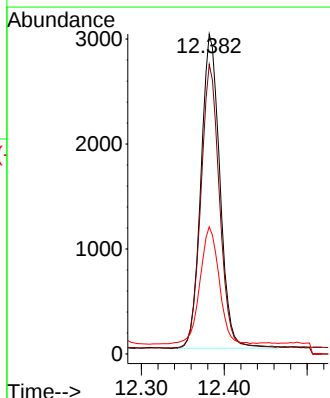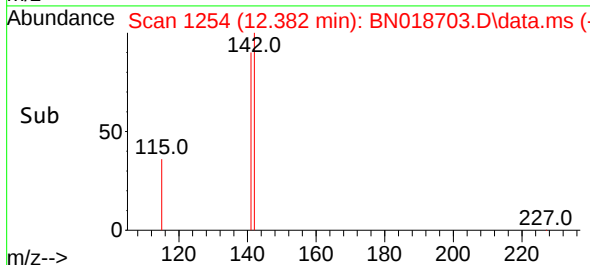

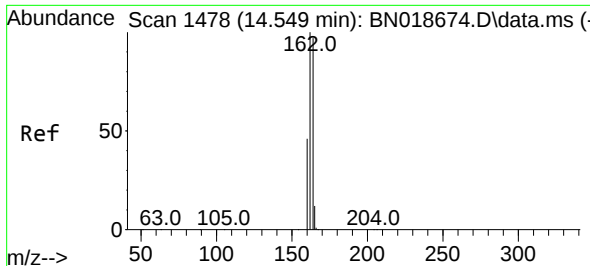

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.549 min Scan# 1478
Delta R.T. -0.000 min
Lab File: BN018703.D
Acq: 23 Feb 2022 18:32




Instrument :
BNA_N
ClientSampleId :
PRPH-1-GW

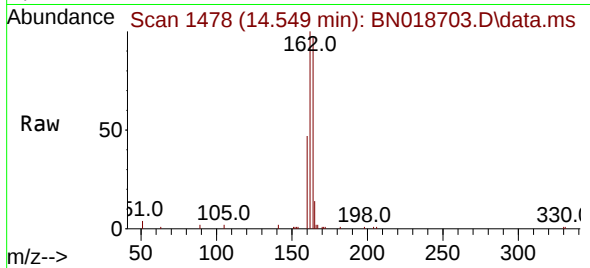


Tgt Ion:164 Resp: 10200
Ion Ratio Lower Upper
164 100
162 103.0 80.2 120.2
160 48.1 36.9 55.3

Manual Integrations
APPROVED



Reviewed By :Yogesh Patel 02/24/2022
Supervised By :mohammad ahmed 02/24/2022

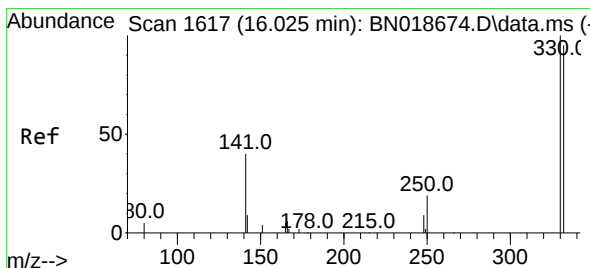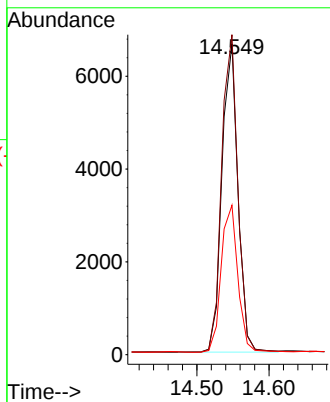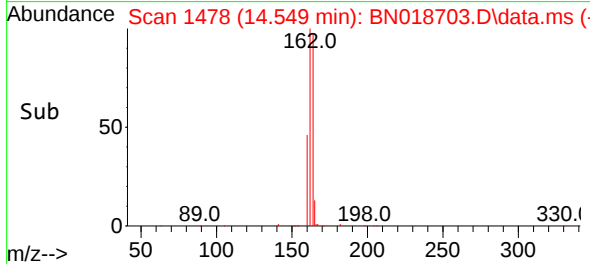


#14
2,4,6-Tribromophenol
Concen: 0.273 ng
RT: 16.025 min Scan# 1617
Delta R.T. 0.000 min
Lab File: BN018703.D
Acq: 23 Feb 2022 18:32

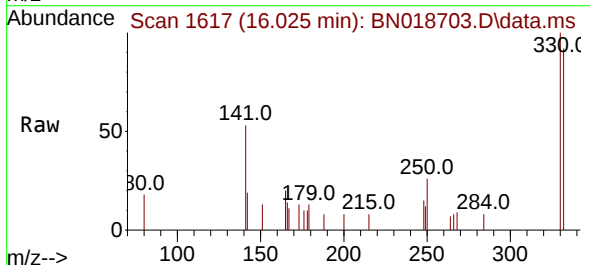


Tgt Ion:330 Resp: 1086
Ion Ratio Lower Upper
330 100
332 95.2 0.0 0.0#
141 40.4 21.3 31.9#

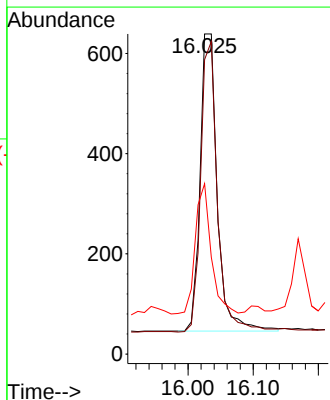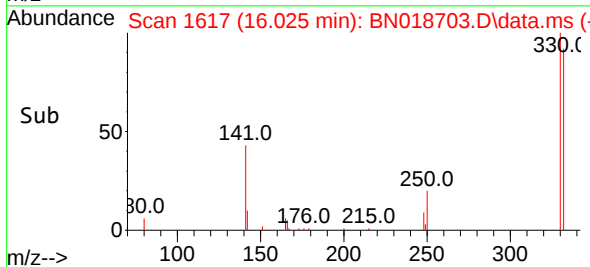

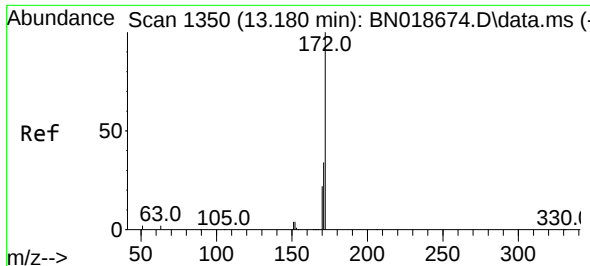

#15
2-Fluorobiphenyl
Concen: 0.262 ng
RT: 13.180 min Scan# 11
Delta R.T. -0.000 min
Lab File: BN018703.D
Acq: 23 Feb 2022 18:32




Instrument :
BNA_N
ClientSampleId :
PRPH-1-GW

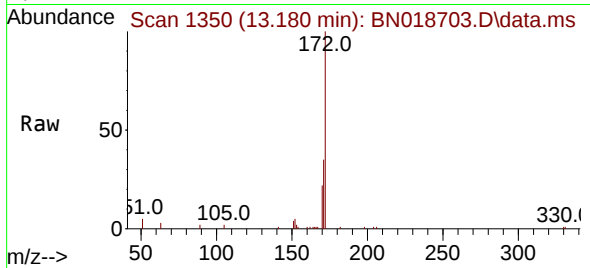

Tgt Ion:172 Resp: 1266
Ion Ratio Lower Upper
172 100
171 34.5 27.4 41.0
170 22.4 18.4 27.6




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 02/24/2022
Supervised By :mohammad ahmed 02/24/2022

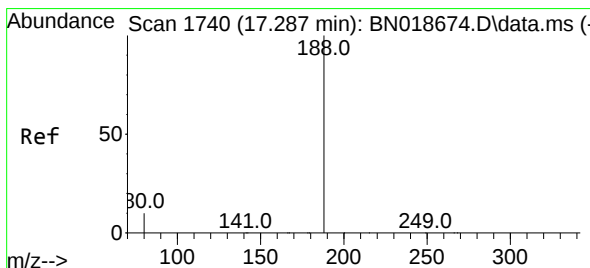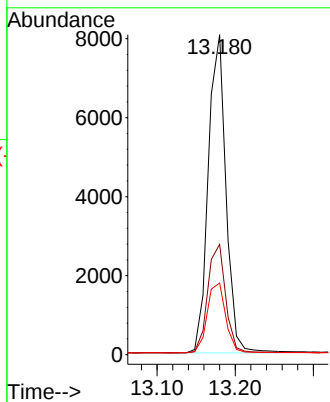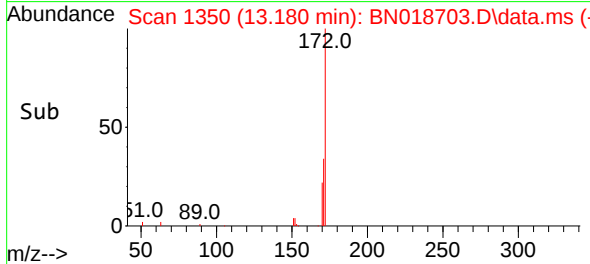

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.287 min Scan# 1740
Delta R.T. -0.000 min
Lab File: BN018703.D
Acq: 23 Feb 2022 18:32


Tgt Ion:188 Resp: 19763
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 9.6 7.0 10.4

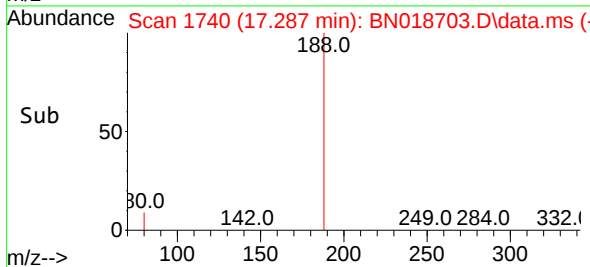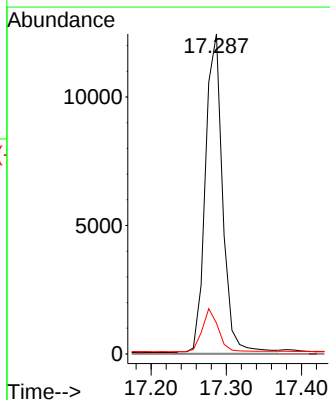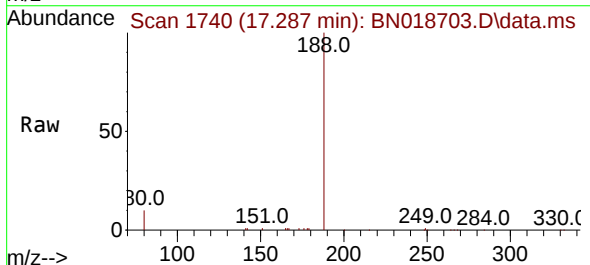

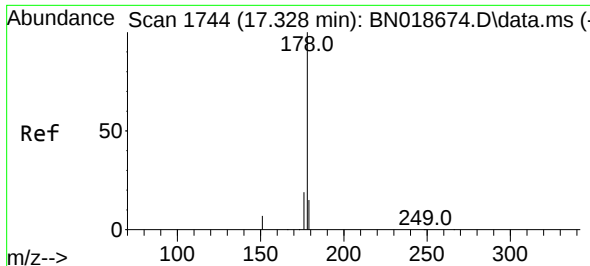

#25
Phenanthrene
Concen: 0.031 ng
RT: 17.328 min Scan# 1744
Delta R.T. -0.000 min
Lab File: BN018703.D
Acq: 23 Feb 2022 18:32




Instrument :
BNA_N
ClientSampleId :
PRPH-1-GW

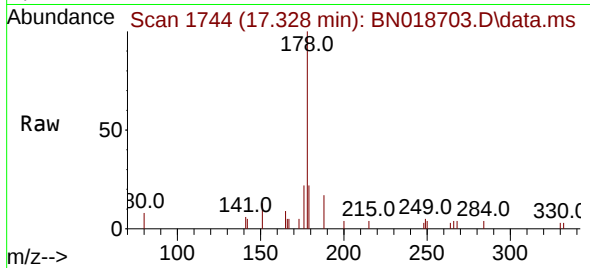

Tgt Ion:178 Resp: 2049
Ion Ratio Lower Upper
178 100
176 21.7 15.3 22.9
179 16.3 12.3 18.5




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 02/24/2022
Supervised By :mohammad ahmed 02/24/2022

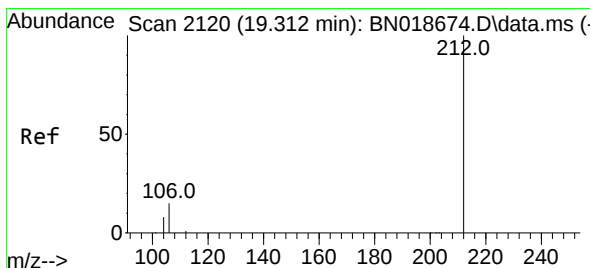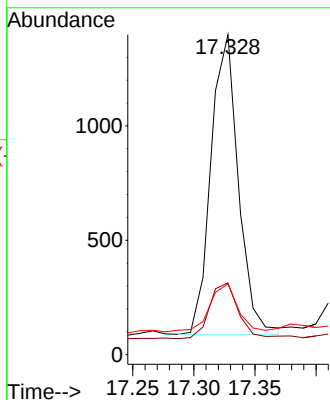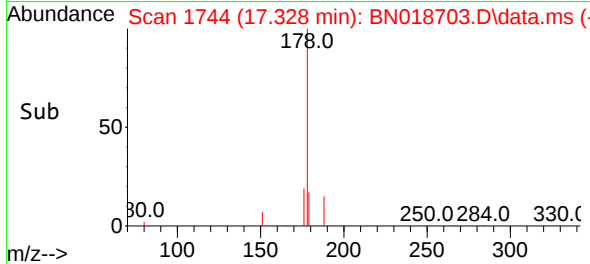

#27
Fluoranthene-d10
Concen: 0.308 ng
RT: 19.312 min Scan# 2120
Delta R.T. -0.000 min
Lab File: BN018703.D
Acq: 23 Feb 2022 18:32


Tgt Ion:212 Resp: 16497
Ion Ratio Lower Upper
212 100
106 15.5 8.4 12.6#
104 8.8 4.5 6.7#

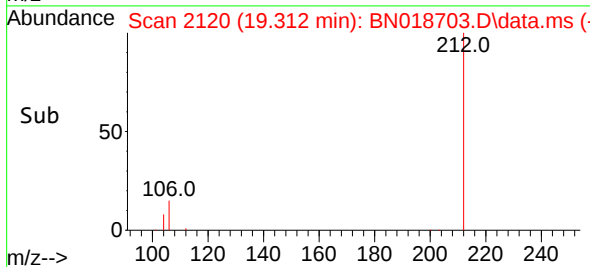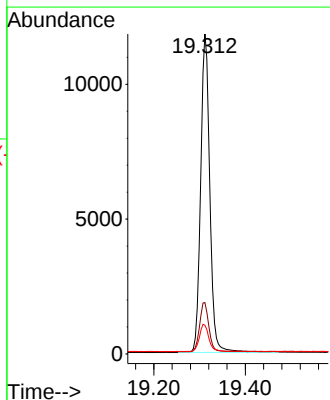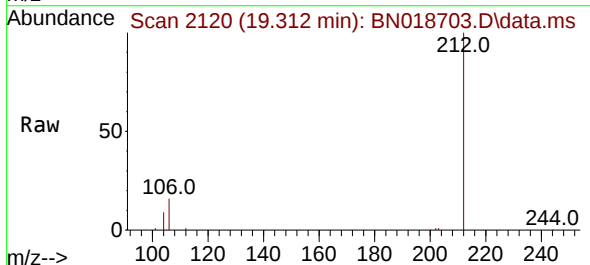

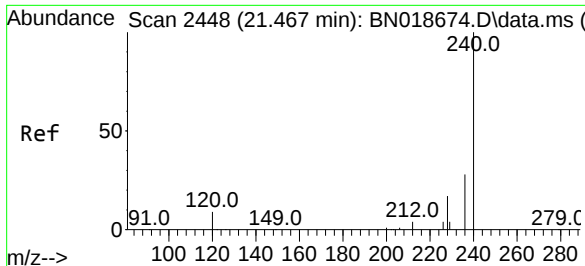

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.467 min Scan# 2448
Delta R.T. -0.000 min
Lab File: BN018703.D
Acq: 23 Feb 2022 18:32




Instrument :
BNA_N
ClientSampleId :
PRPH-1-GW

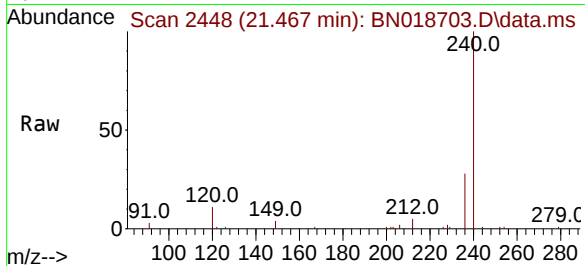

Tgt Ion:240 Resp: 13689
Ion Ratio Lower Upper
240 100
120 10.9 6.0 9.0#
236 27.6 21.4 32.2




Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 02/24/2022
Supervised By :mohammad ahmed 02/24/2022

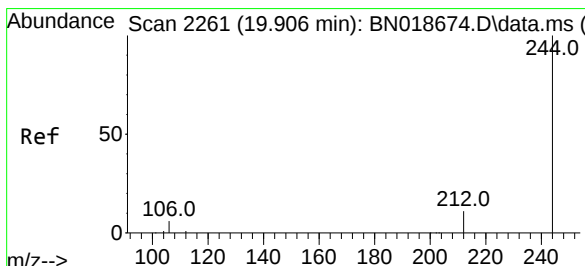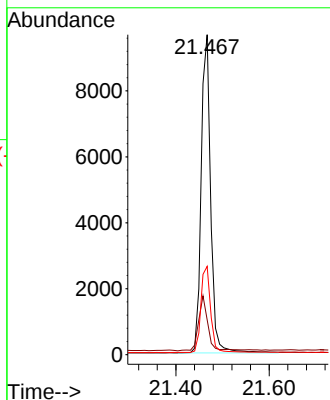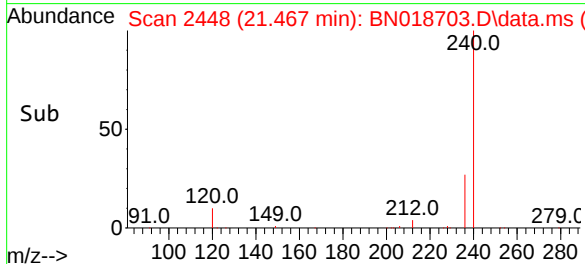

#31
Terphenyl-d14
Concen: 0.370 ng
RT: 19.906 min Scan# 2261
Delta R.T. -0.000 min
Lab File: BN018703.D
Acq: 23 Feb 2022 18:32

Tgt Ion:244 Resp: 10997
Ion Ratio Lower Upper
244 100
212 10.3 6.2 9.2#
122 0.0 7.9 11.9#

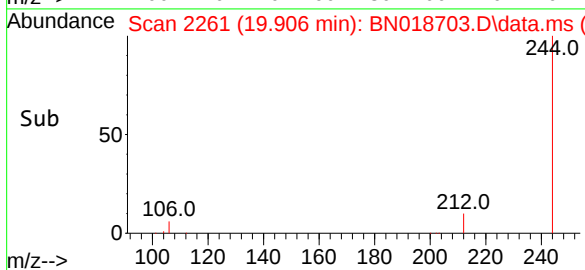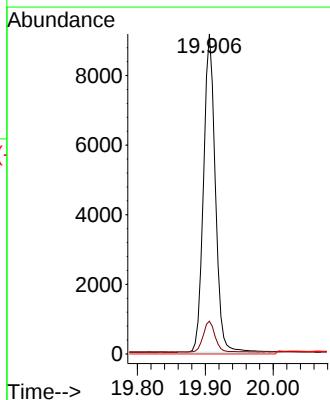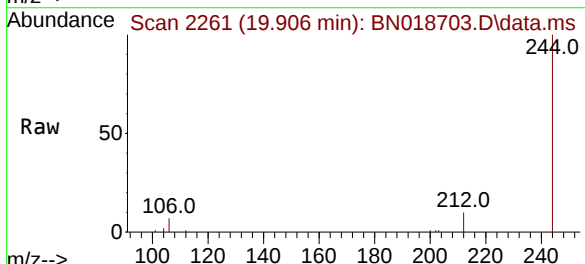

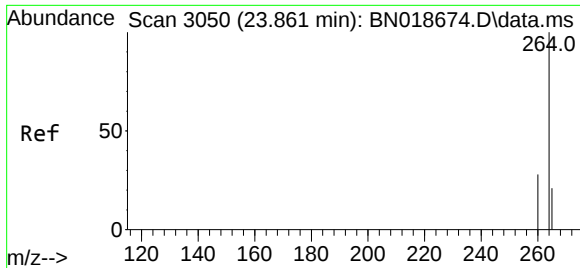

#35

Perylene-d12

Concen: 0.400 ng

RT: 23.860 min Scan# 30

Delta R.T. -0.000 min

Lab File: BN018703.D


Acq: 23 Feb 2022 18:32

Instrument :

BNA_N

ClientSampleId :

PRPH-1-GW

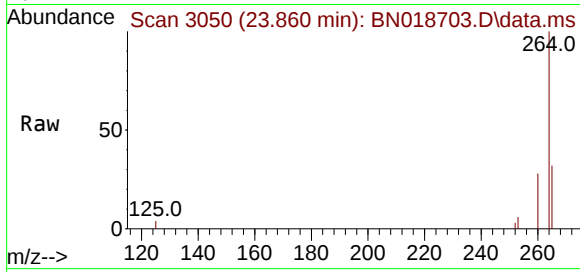

Tgt Ion:264 Resp: 1118

Ion Ratio Lower Upper

264 100

260 28.4 20.2 30.4

265 32.5 18.2 27.2

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 02/24/2022

Supervised By :mohammad ahmed 02/24/2022

