
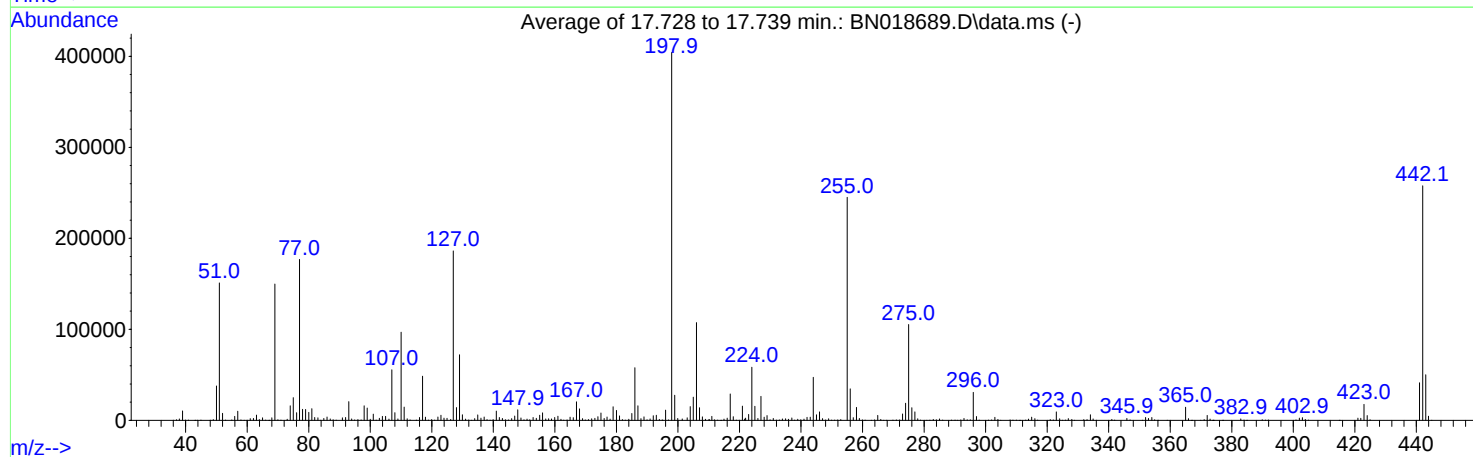


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022322\
 Data File : BN018689.D
 Acq On : 23 Feb 2022 09:54
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN022222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Feb 22 16:23:51 2022

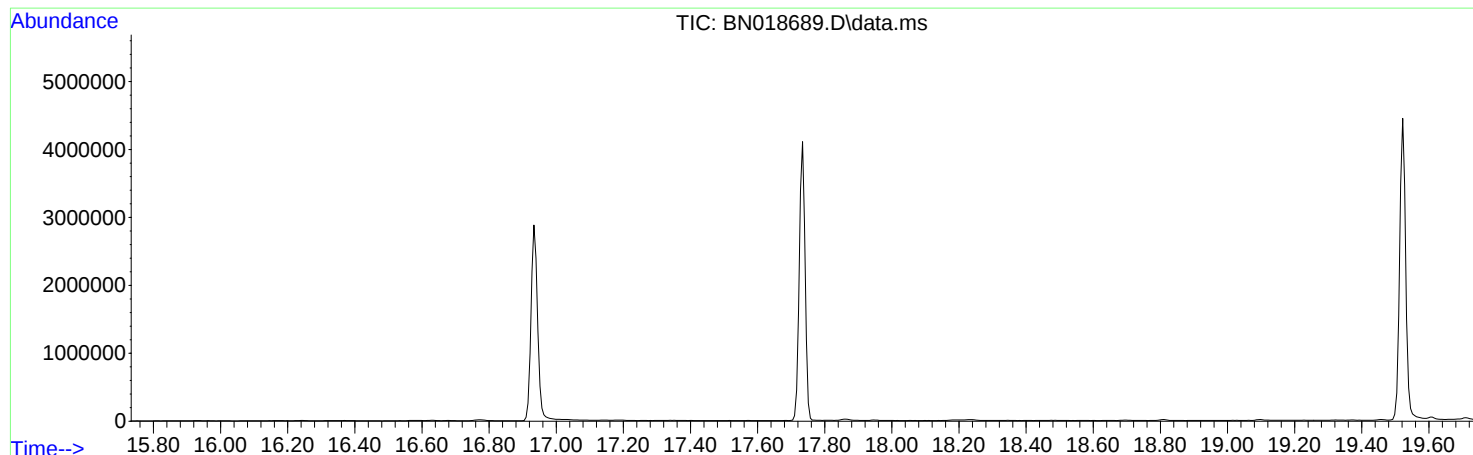

AutoFind: Scans 2506, 2507, 2508; Background Corrected with Scan 2499

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.4	151027	PASS
68	69	0.00	2	1.8	2750	PASS
69	198	0.00	100	37.1	149780	PASS
70	69	0.00	2	0.5	754	PASS
127	198	10	80	46.1	186240	PASS
197	198	0.00	2	0.1	578	PASS
198	198	100	100	100.0	404181	PASS
199	198	5	9	6.8	27653	PASS
275	198	10	60	26.0	105253	PASS
365	198	1	100	3.6	14505	PASS
441	198	0.01	100	10.2	41275	PASS
442	442	50	100	100.0	257792	PASS
443	442	15	24	19.5	50203	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
2/23/2022	BNA_N	<u>BN018689.D</u>
Compound Name	Response	Retention Time
DDT	1233501	20.76
DDD	13045	20.32
DDE	635	19.81
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13680	1247181	1.10

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022322\
Data File : BN018689.D
Acq On : 23 Feb 2022 09:54
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Feb 23 14:23:18 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 23 14:23:13 2022
Response via : Initial Calibration

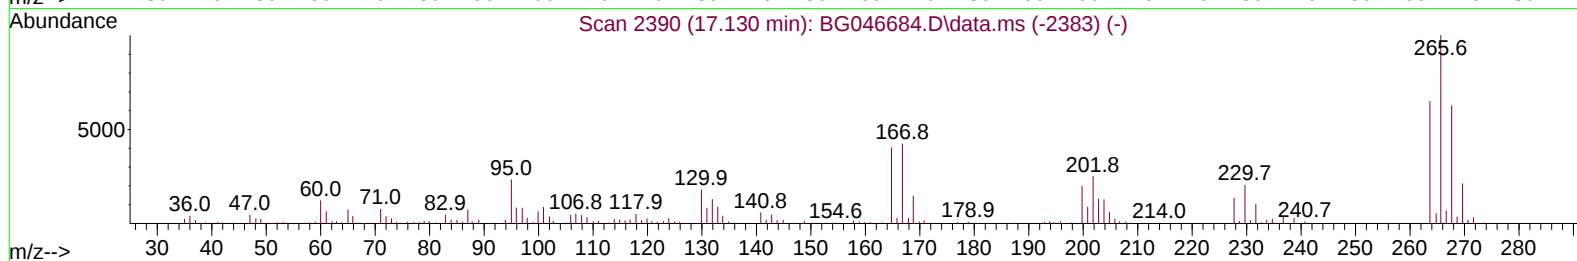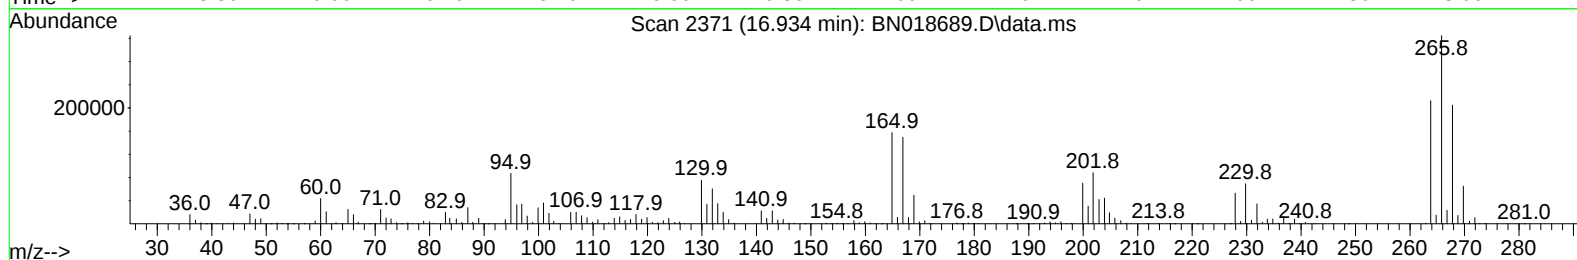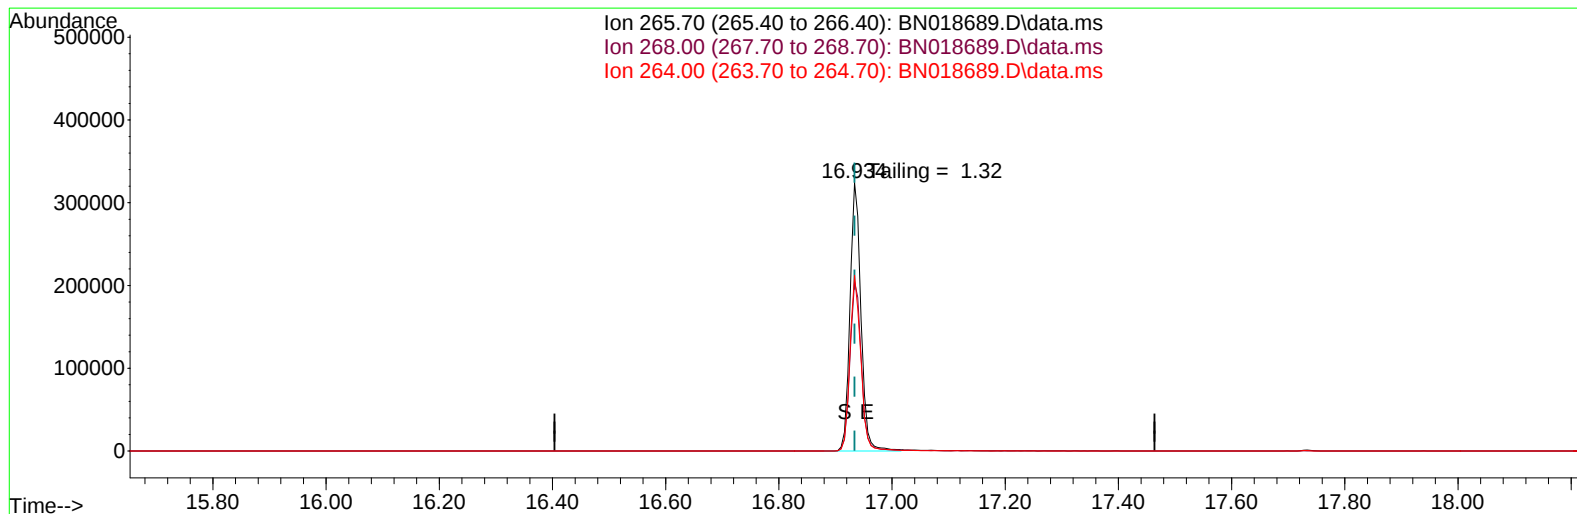

TIC: BN018689.D\data.ms

(70) Pentachlorophenol (C)

16.934min (0.000) 19903.77 ng




response 439390

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.09
264.00	61.60	65.44
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022322\
Data File : BN018689.D
Acq On : 23 Feb 2022 09:54
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Feb 23 14:23:18 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 23 14:23:13 2022
Response via : Initial Calibration

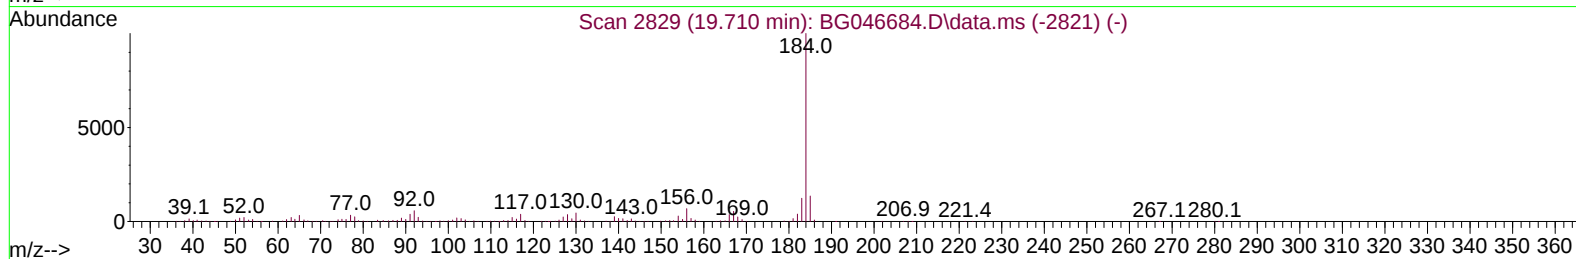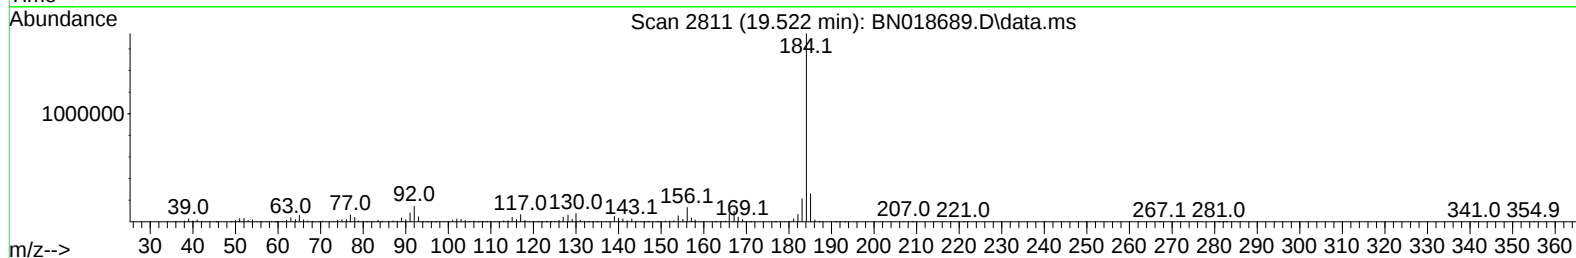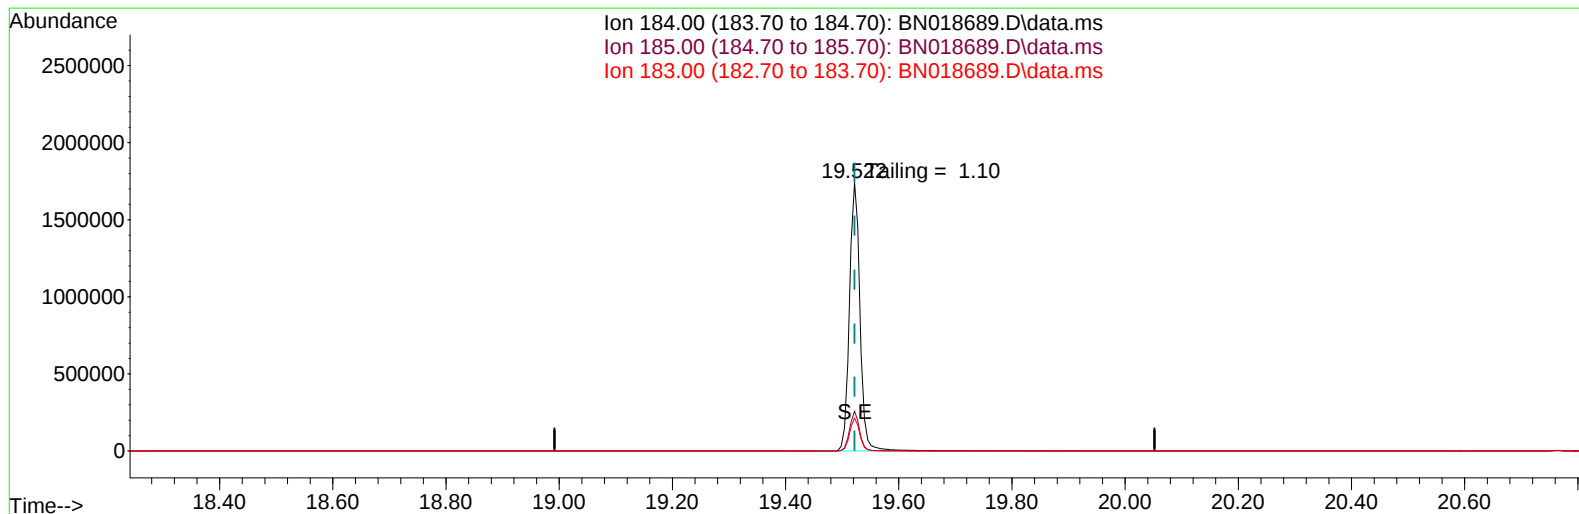

TIC: BN018689.D\data.ms

(77) Benzidine

19.522min (0.000) 0.00 ng

response 2260058

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.91
183.00	13.20	12.30
0.00	0.00	0.00