


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022323\
 Data File : BN024090.D
 Acq On : 22 Feb 2023 16:40
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN020723.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Feb 23 03:52:37 2023

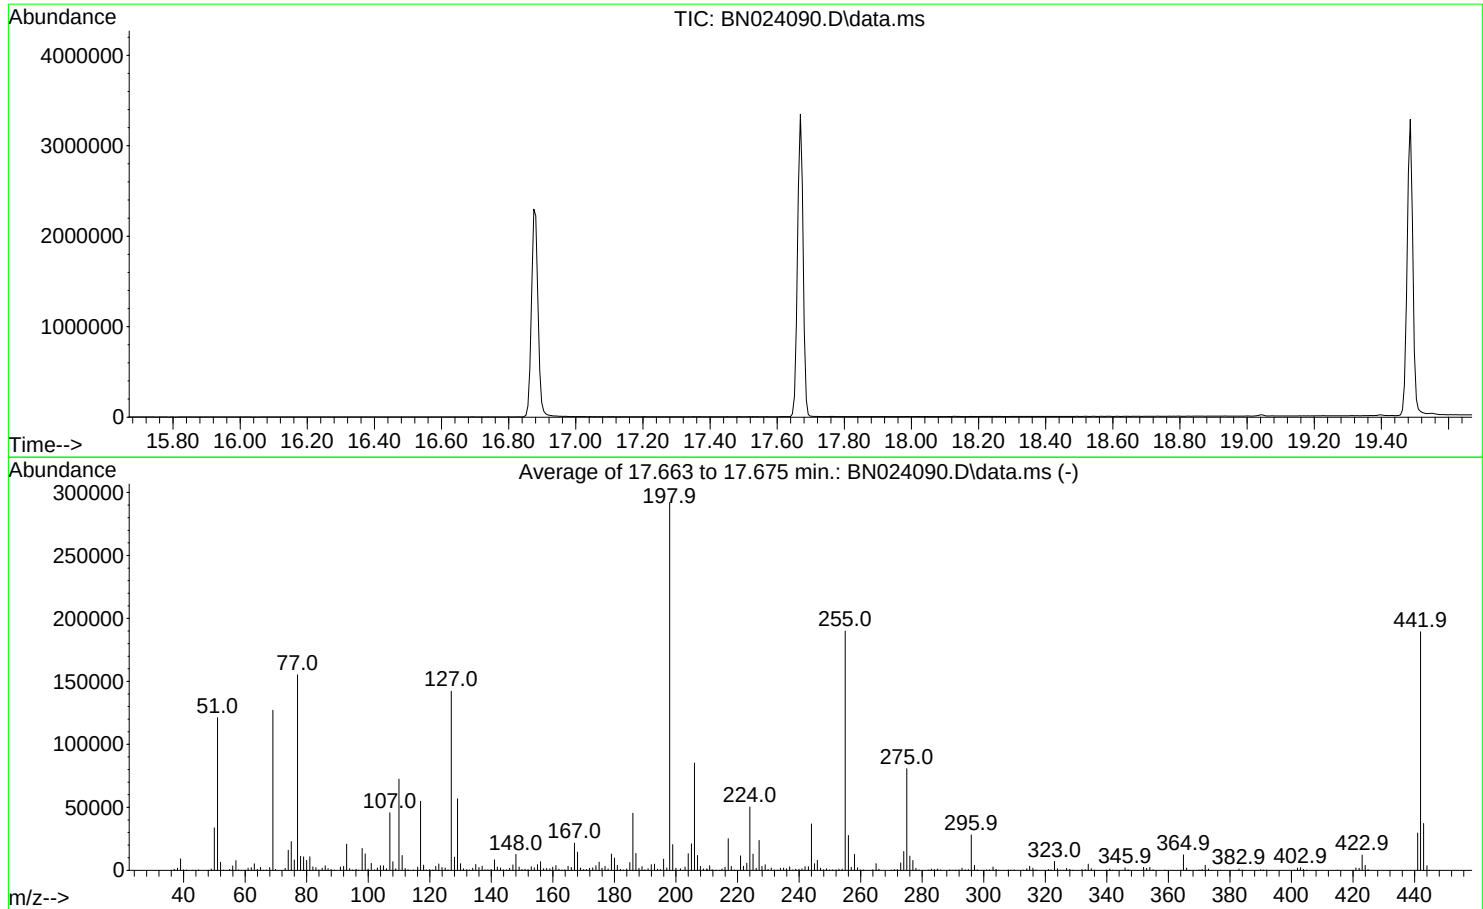




AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.5	121133	PASS
68	69	0.00	2	1.7	2174	PASS
69	198	0.00	100	43.5	127189	PASS
70	69	0.00	2	0.6	744	PASS
127	198	10	80	48.7	142277	PASS
197	198	0.00	2	0.6	1890	PASS
198	198	100	100	100.0	292117	PASS
199	198	5	9	7.0	20435	PASS
275	198	10	60	27.6	80629	PASS
365	198	1	100	4.2	12332	PASS
441	198	0.01	100	10.1	29592	PASS
442	442	50	100	100.0	189349	PASS
443	442	15	24	19.6	37133	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022323\
Data File : BN024090.D
Acq On : 22 Feb 2023 16:40
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Feb 23 04:28:30 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 23 04:28:27 2023
Response via : Initial Calibration

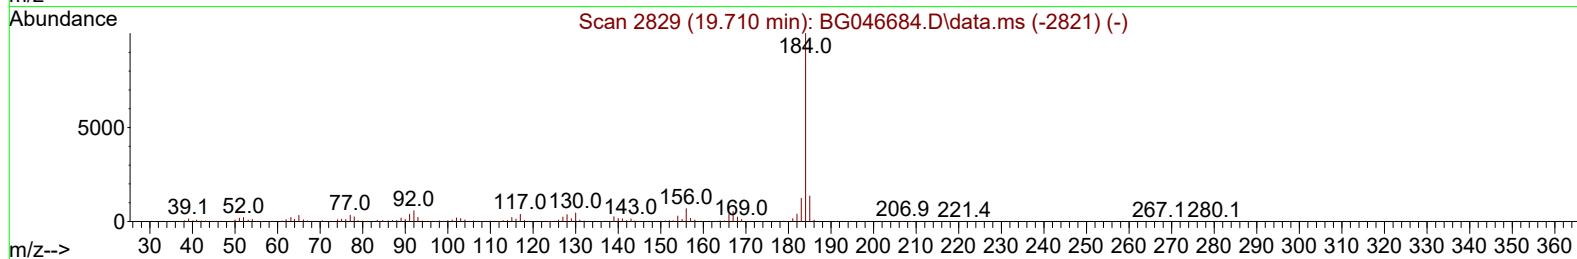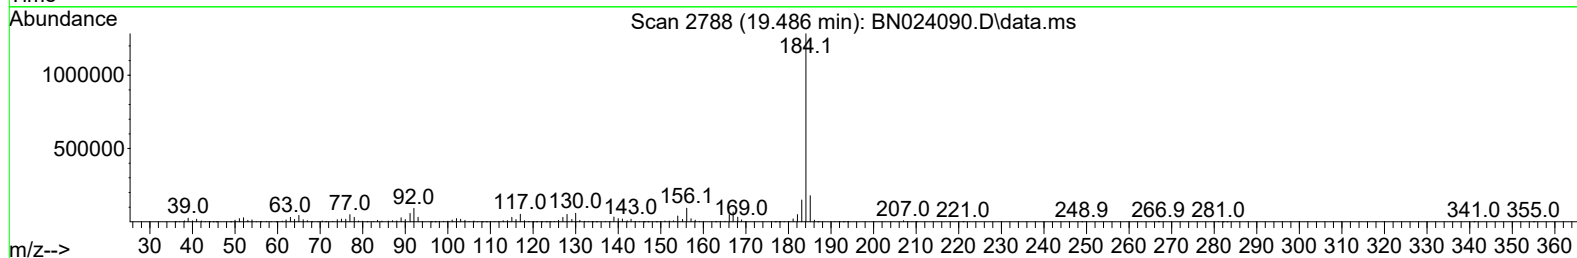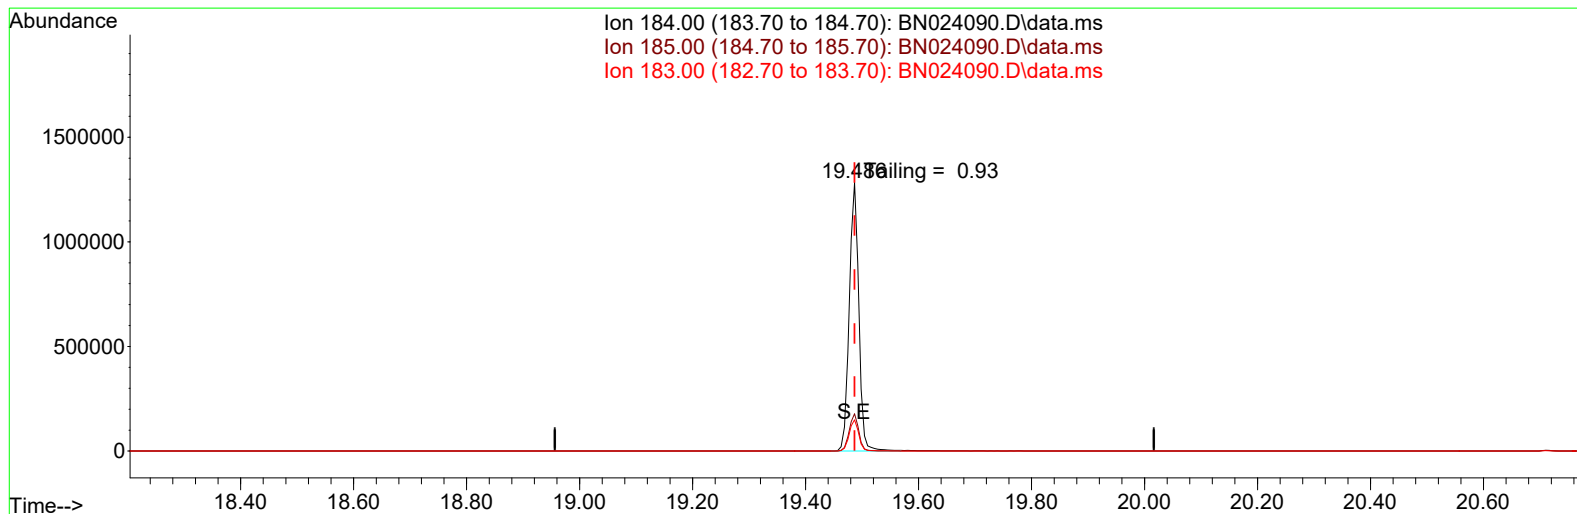

TIC: BN024090.D\data.ms

(77) Benzidine

19.486min (0.000) 0.00 ng

response 1509752

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.91
183.00	13.20	11.63
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/23/2023	BNA_N	<u>BN024090.D</u>
Compound Name	Response	Retention Time
DDT	854013	20.716
DDD	11335	20.275
DDE	805	19.769
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12140	866153	1.40

Instrument :
BNA_N
ClientSampleId :
DFTPP