


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022323\
 Data File : BN024097.D
 Acq On : 23 Feb 2023 12:59
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN020723.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Feb 23 03:52:37 2023

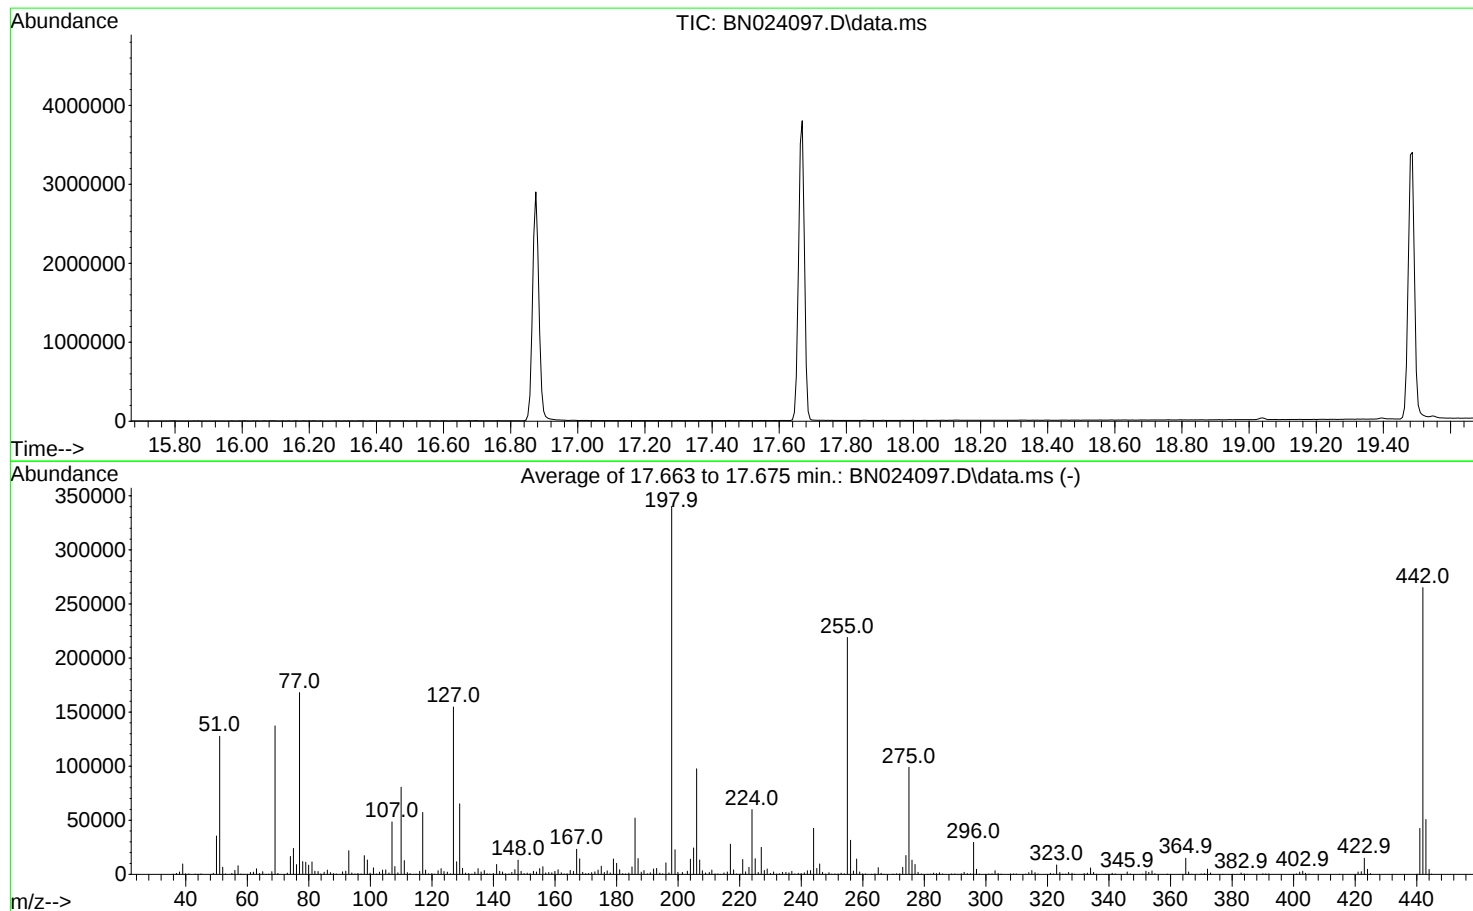




AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.5	127587	PASS
68	69	0.00	2	1.8	2480	PASS
69	198	0.00	100	40.4	137320	PASS
70	69	0.00	2	0.6	782	PASS
127	198	10	80	45.5	154765	PASS
197	198	0.00	2	0.4	1326	PASS
198	198	100	100	100.0	340203	PASS
199	198	5	9	6.7	22794	PASS
275	198	10	60	29.1	98923	PASS
365	198	1	100	4.4	14934	PASS
441	198	0.01	100	12.5	42456	PASS
442	442	50	100	100.0	265131	PASS
443	442	15	24	19.1	50720	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022323\
Data File : BN024097.D
Acq On : 23 Feb 2023 12:59
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Feb 24 03:43:41 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 24 03:43:37 2023
Response via : Initial Calibration

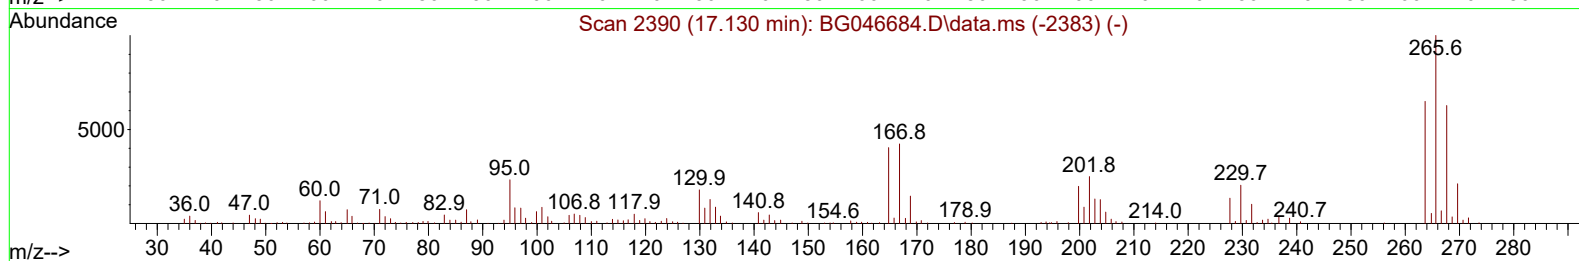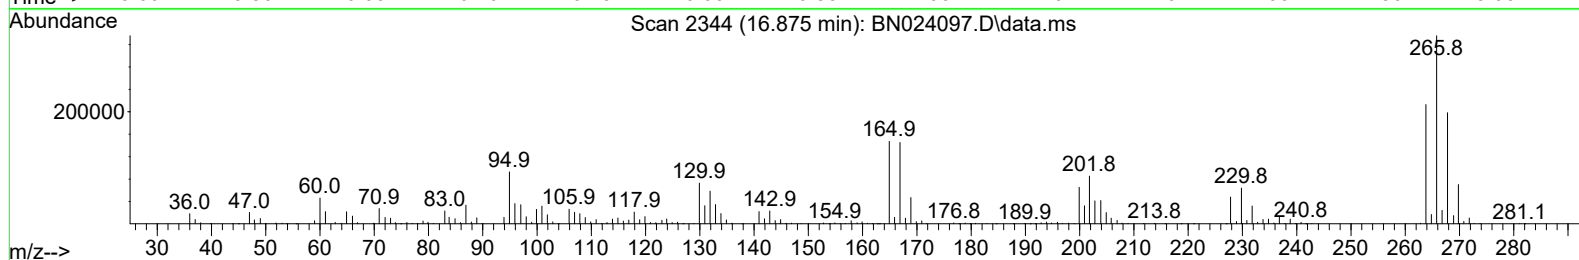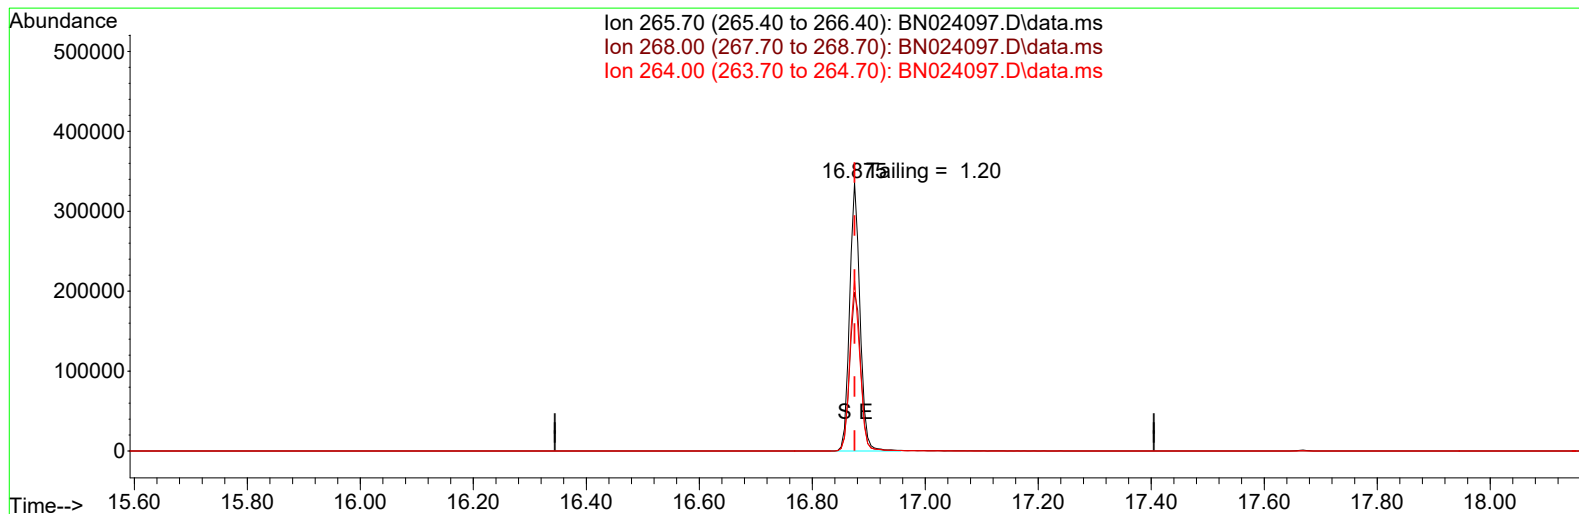

TIC: BN024097.D\data.ms

(70) Pentachlorophenol (C)

16.875min (0.000) 19463.05 ng




response 430119

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	59.08
264.00	61.60	63.39
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022323\
 Data File : BN024097.D
 Acq On : 23 Feb 2023 12:59
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Feb 24 03:43:41 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 24 03:43:37 2023
 Response via : Initial Calibration

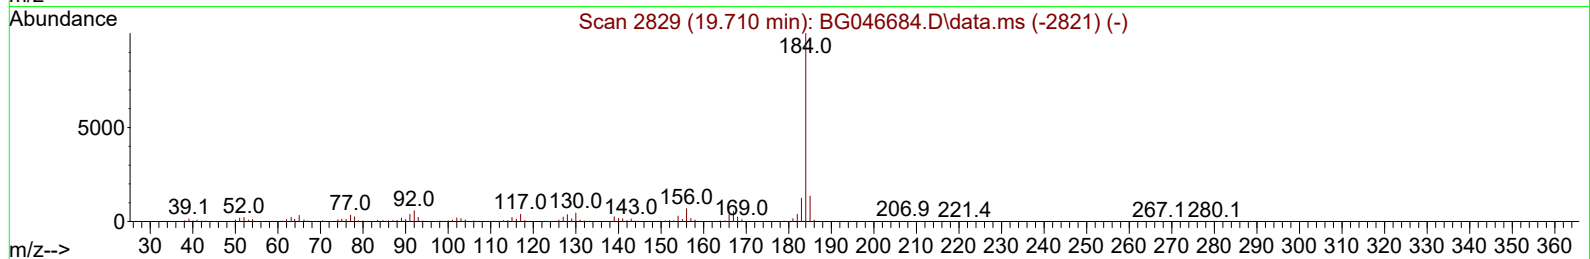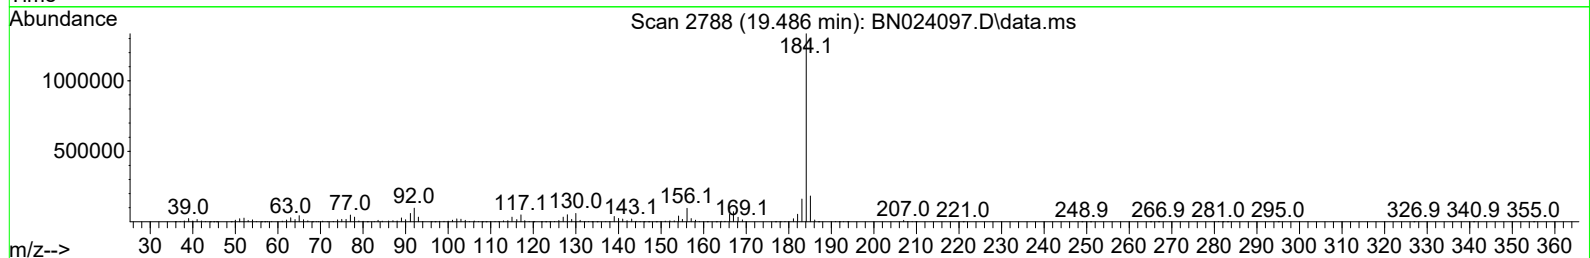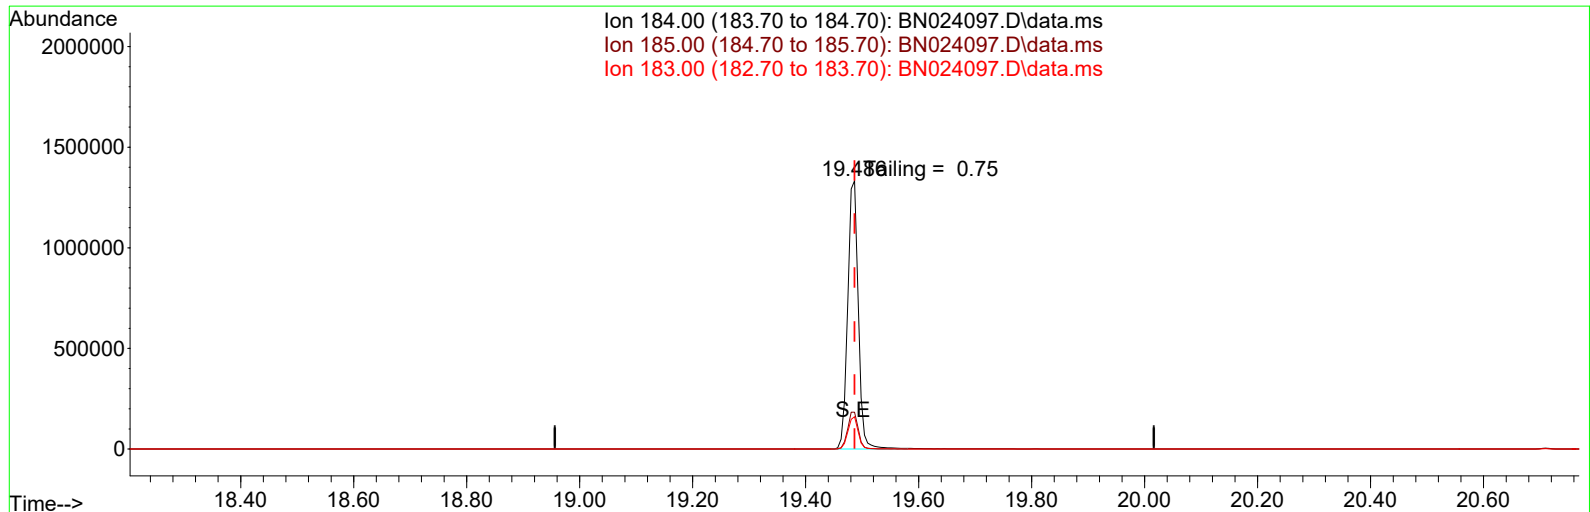

TIC: BN024097.D\data.ms

(77) Benzidine

19.486min (0.000) 0.00 ng

response 1740090

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.72
183.00	13.20	12.08
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/23/2023	BNA_N	<u>BN024097.D</u>
Compound Name	Response	Retention Time
DDT	984856	20.71
DDD	14902	20.275
DDE	1035	19.763
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15937	1000793	1.59

Instrument :
BNA_N
ClientSampleId :
DFTPP