
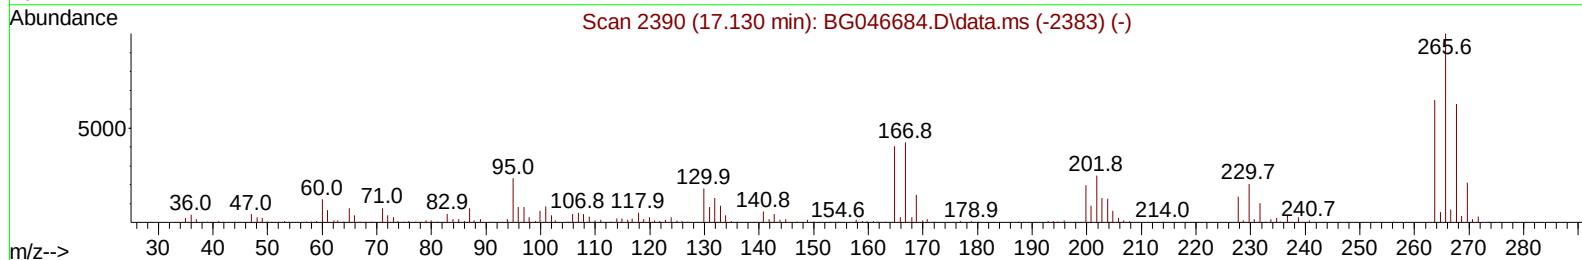
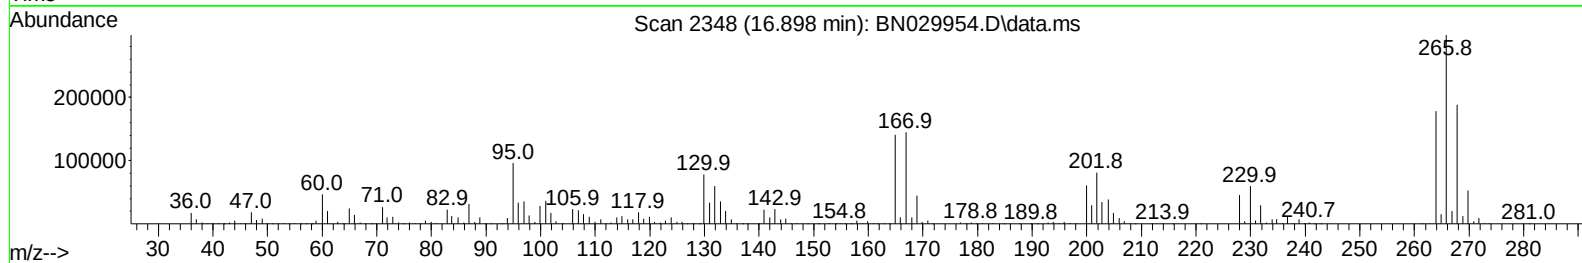


Quant Time: Feb 24 05:20:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 24 05:20:21 2024
Response via : Initial Calibration

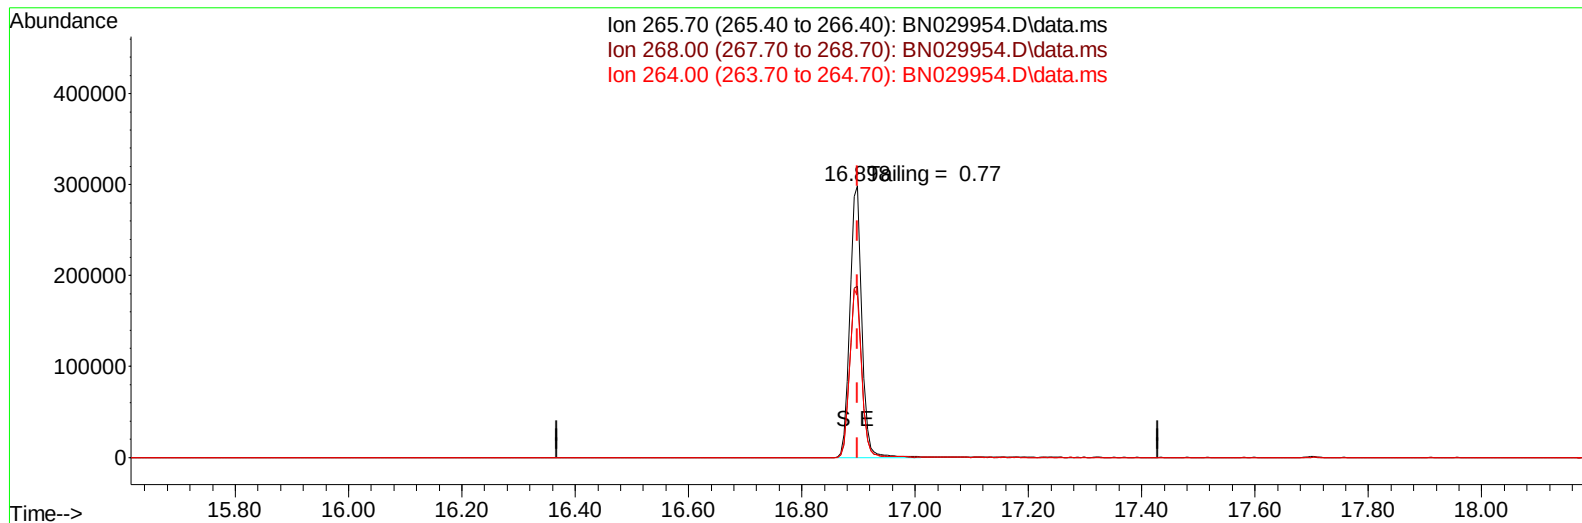

TIC: BN029954.D\data.ms

(70) Pentachlorophenol (C)




16.898min (0.000) 23871.33 ng

response 440802

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.16
264.00	61.60	59.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022324\
Data File : BN029954.D
Acq On : 23 Feb 2024 13:39
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 24 05:20:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 24 05:20:21 2024
Response via : Initial Calibration

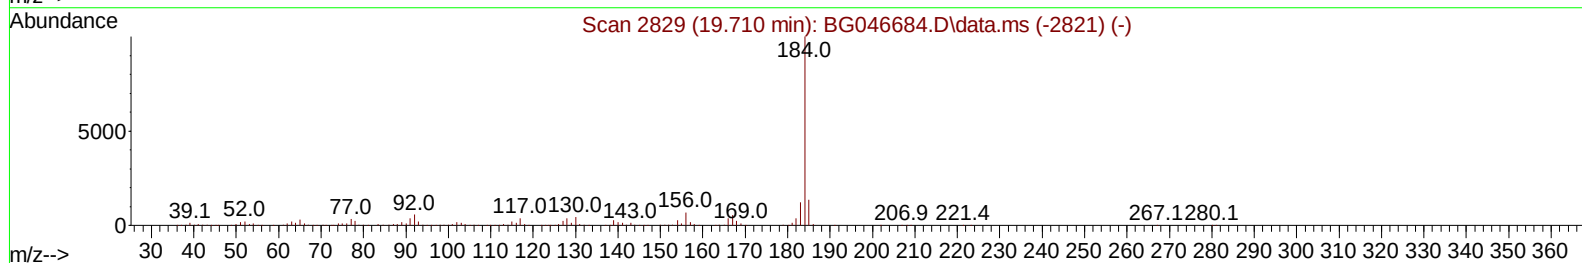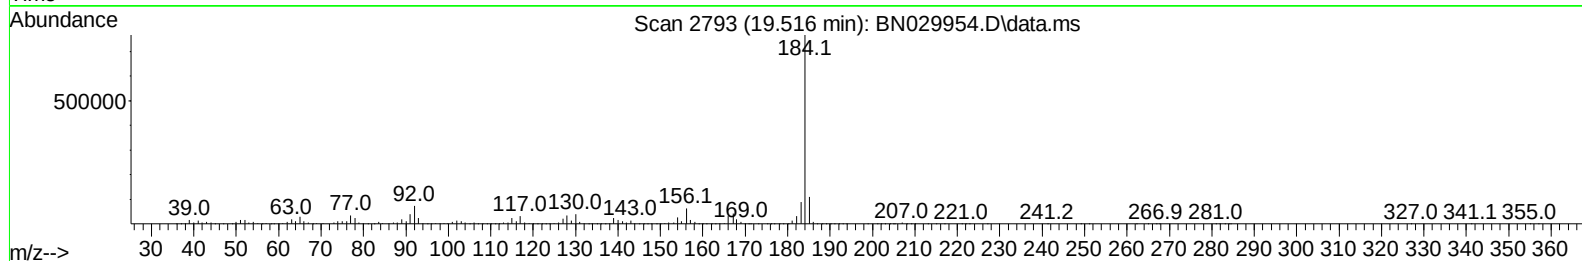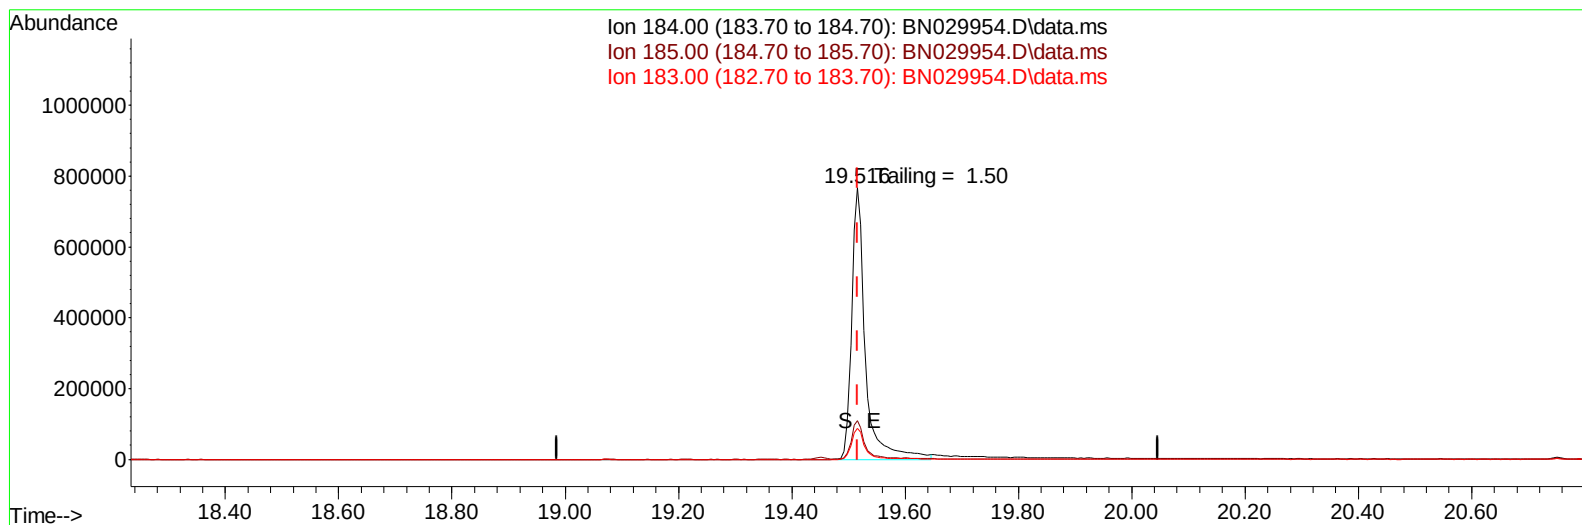

TIC: BN029954.D\data.ms

(77) Benzidine

19.516min (0.000) 195402.16 ng

response 1295019

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.39
183.00	13.20	11.57
0.00	0.00	0.00