
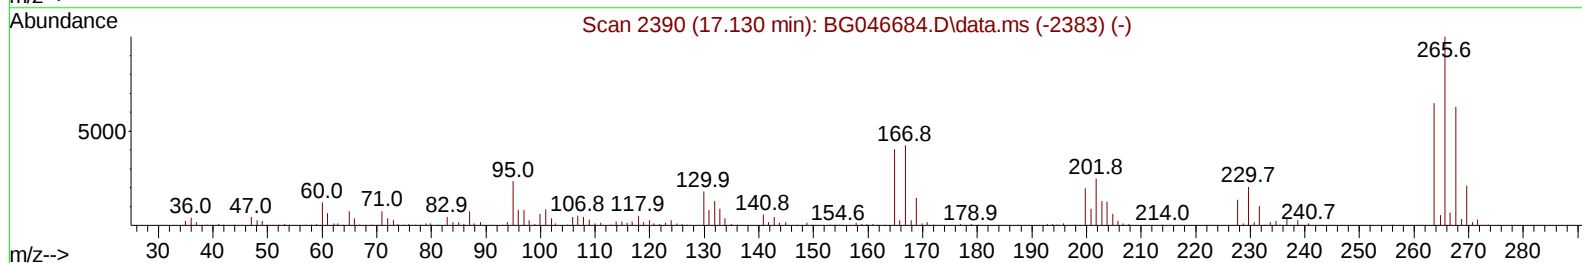
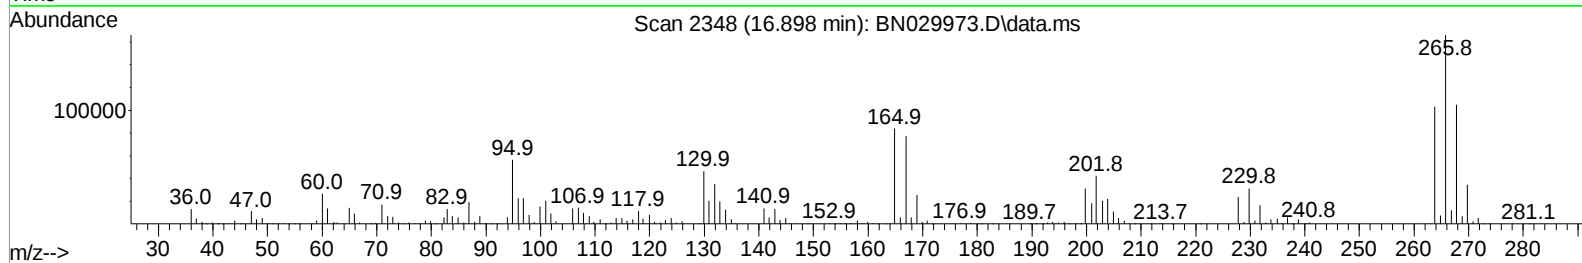


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022324\
Data File : BN029973.D
Acq On : 24 Feb 2024 02:16
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 21 Sample Multiplier: 1

Quant Time: Feb 24 05:21:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 24 05:20:21 2024
Response via : Initial Calibration

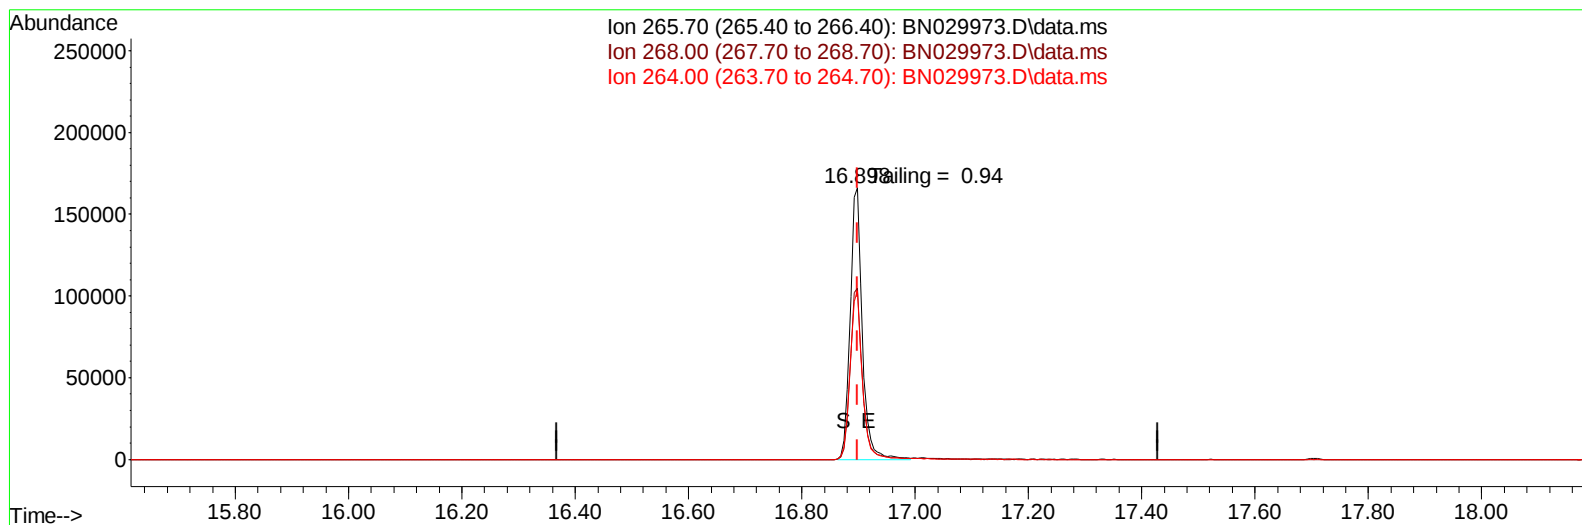




TIC: BN029973.D\data.ms

(70) Pentachlorophenol (C)**16.898min (0.000) 18620.64 ng****response 249298**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.15
264.00	61.60	62.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022324\
Data File : BN029973.D
Acq On : 24 Feb 2024 02:16
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 21 Sample Multiplier: 1

Quant Time: Feb 24 05:21:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 24 05:20:21 2024
Response via : Initial Calibration

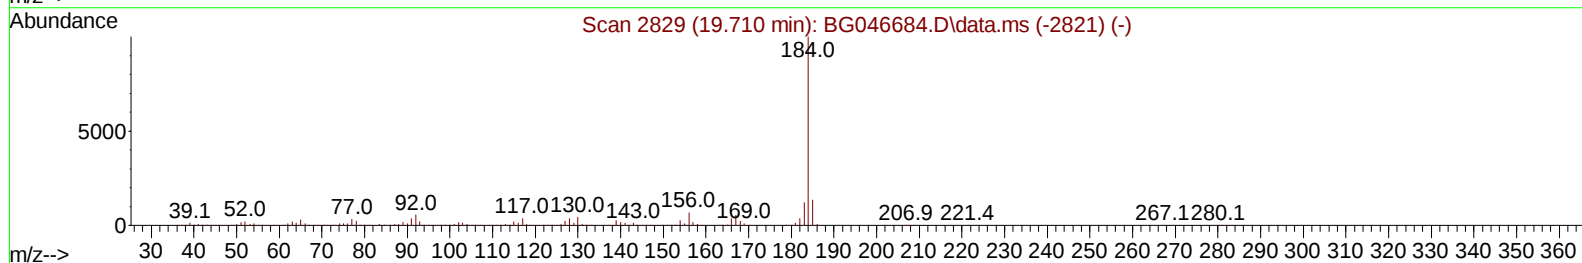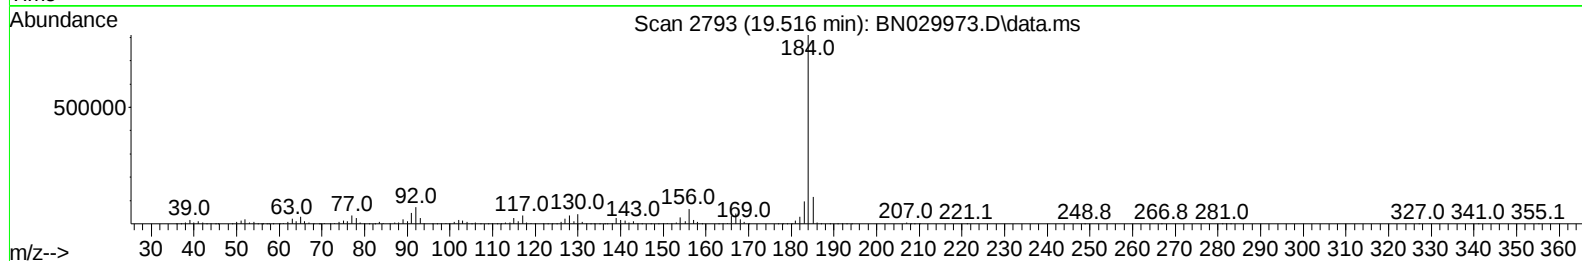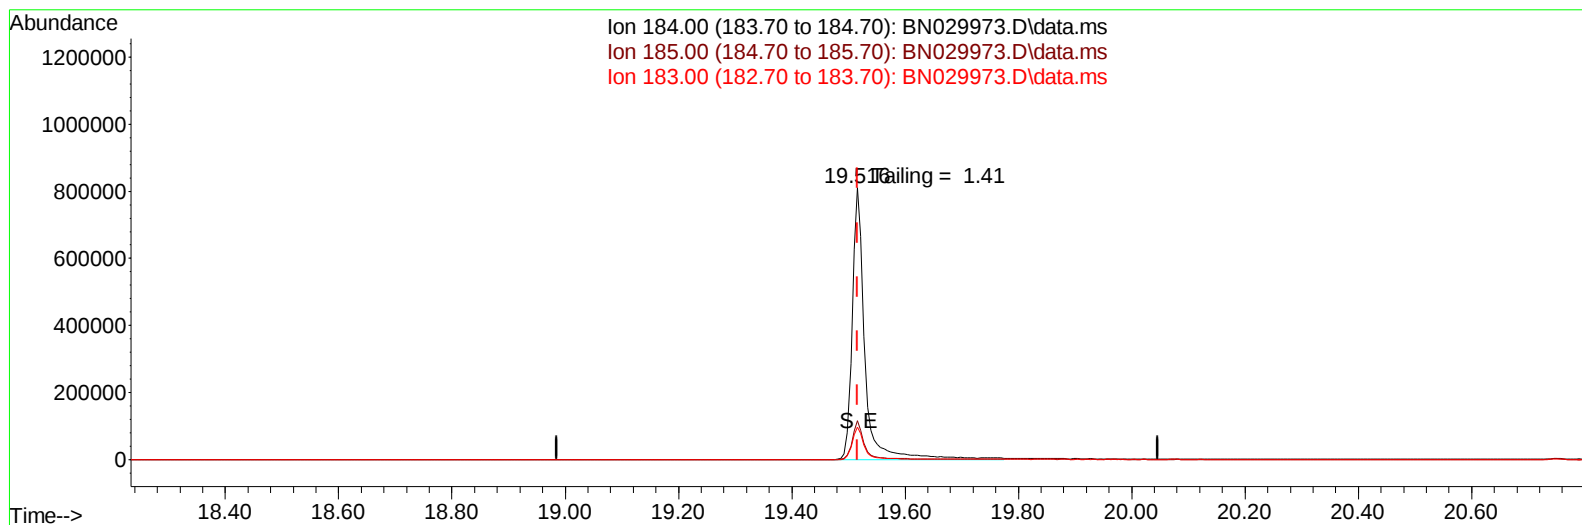

TIC: BN029973.D\data.ms

(77) Benzidine**19.516min (0.000) 0.00 ng****response 1258952**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.18
183.00	13.20	11.97
0.00	0.00	0.00