
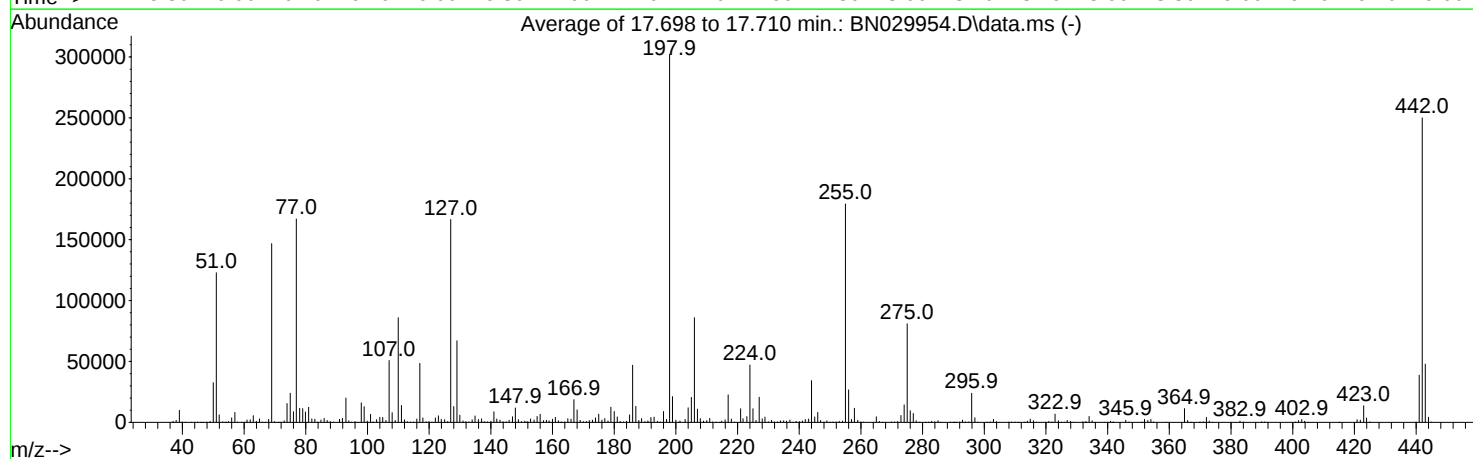


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022324\
Data File : BN029954.D
Acq On : 23 Feb 2024 13:39
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN012924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Feb 26 02:39:45 2024

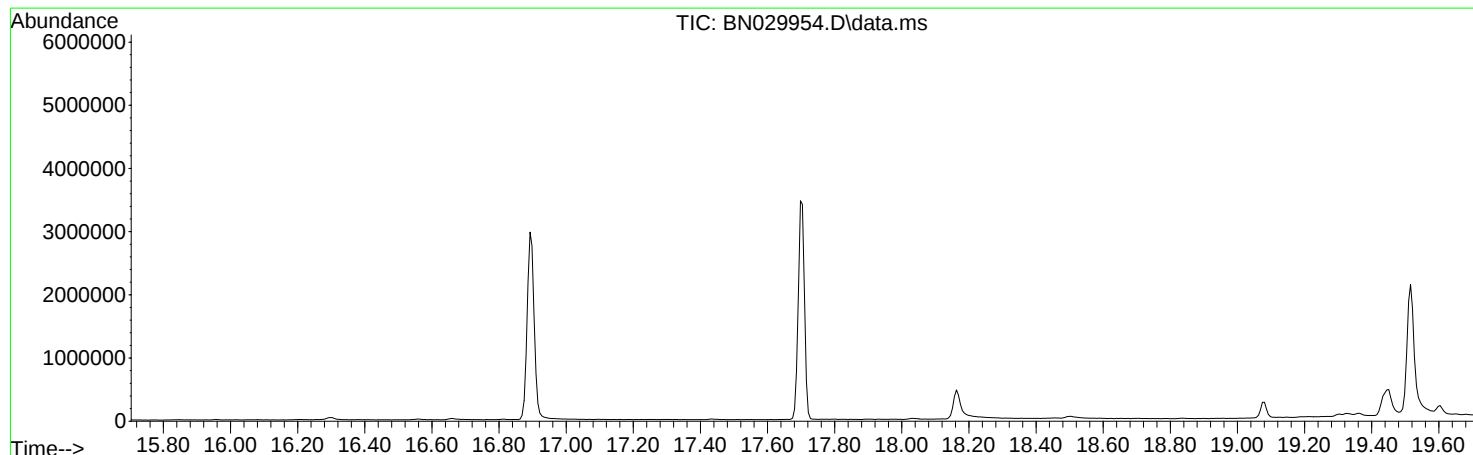




AutoFind: Scans 2484, 2485, 2486; Background Corrected with Scan 2476

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.7	122877	PASS
68	69	0.00	2	1.7	2487	PASS
69	198	0.00	100	48.6	146761	PASS
70	69	0.00	2	0.5	674	PASS
127	198	10	80	55.1	166563	PASS
197	198	0.00	2	0.8	2479	PASS
198	198	100	100	100.0	302037	PASS
199	198	5	9	7.0	21163	PASS
275	198	10	60	26.8	80891	PASS
365	198	1	100	3.7	11303	PASS
441	198	0.01	100	12.8	38763	PASS
442	442	50	100	100.0	250069	PASS
443	442	15	24	19.1	47888	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022324\
Data File : BN029954.D
Acq On : 23 Feb 2024 13:39
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Feb 24 05:20:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 24 05:20:21 2024
Response via : Initial Calibration

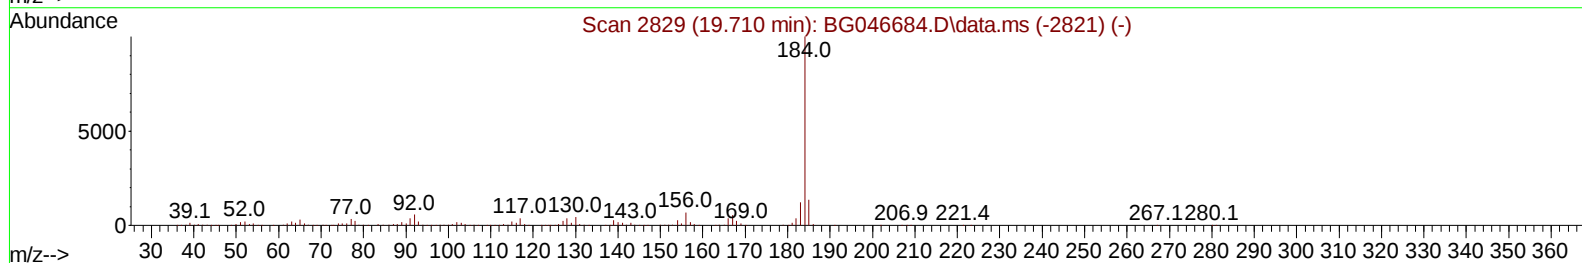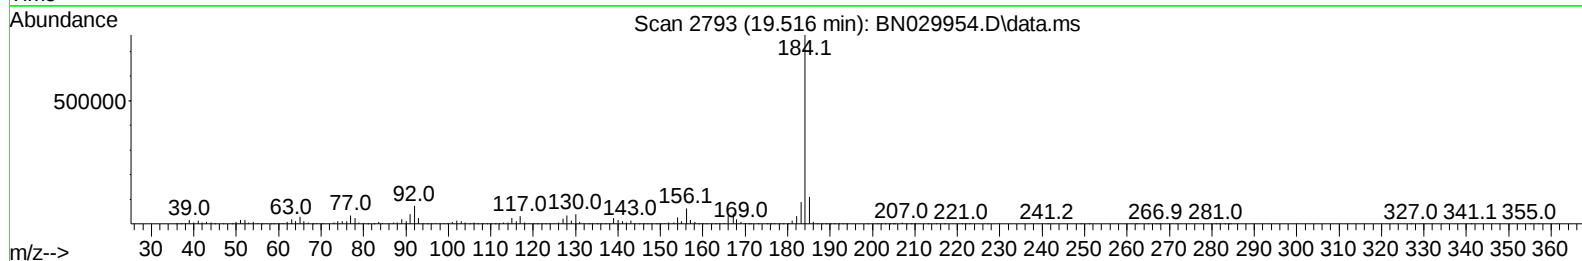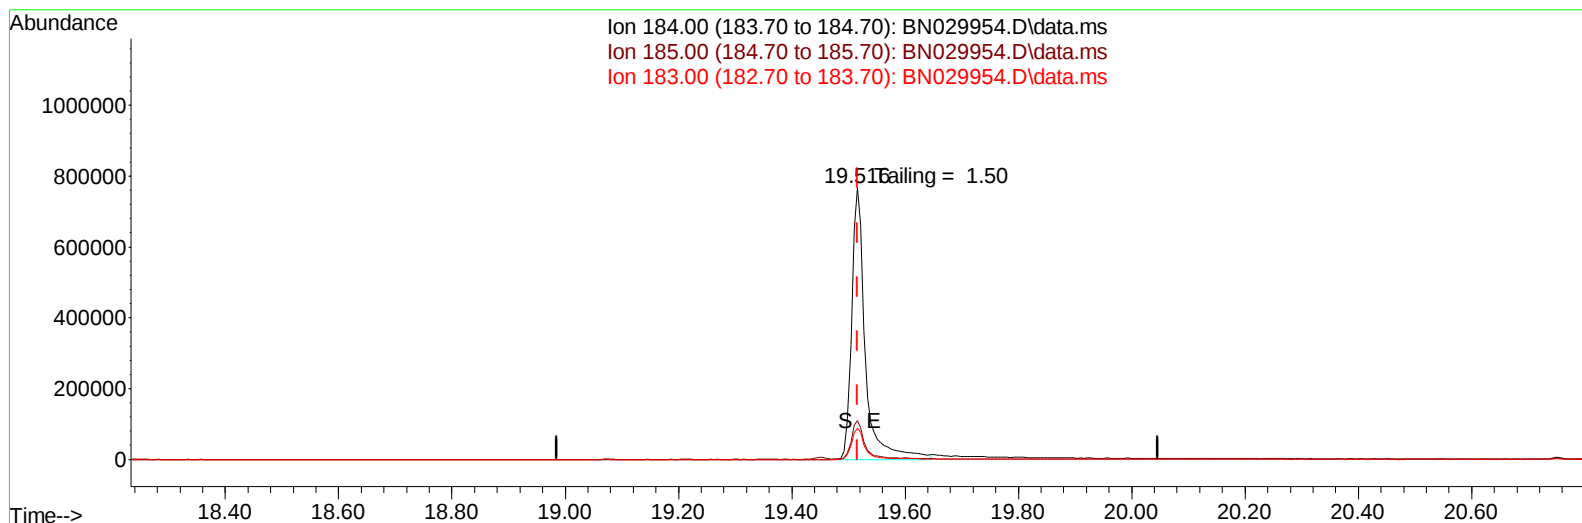

TIC: BN029954.D\data.ms

(77) Benzidine

19.516min (0.000) 195402.16 ng

response 1295019

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.39
183.00	13.20	11.57
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/23/2024	BNA_N	<u>BN029954.D</u>
Compound Name	Response	Retention Time
DDT	1214194	20.751
DDD	19514	20.357
DDE	498	19.075
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
20012	1234206	1.62

Instrument :
BNA_N
ClientSampleId :
DFTPP