
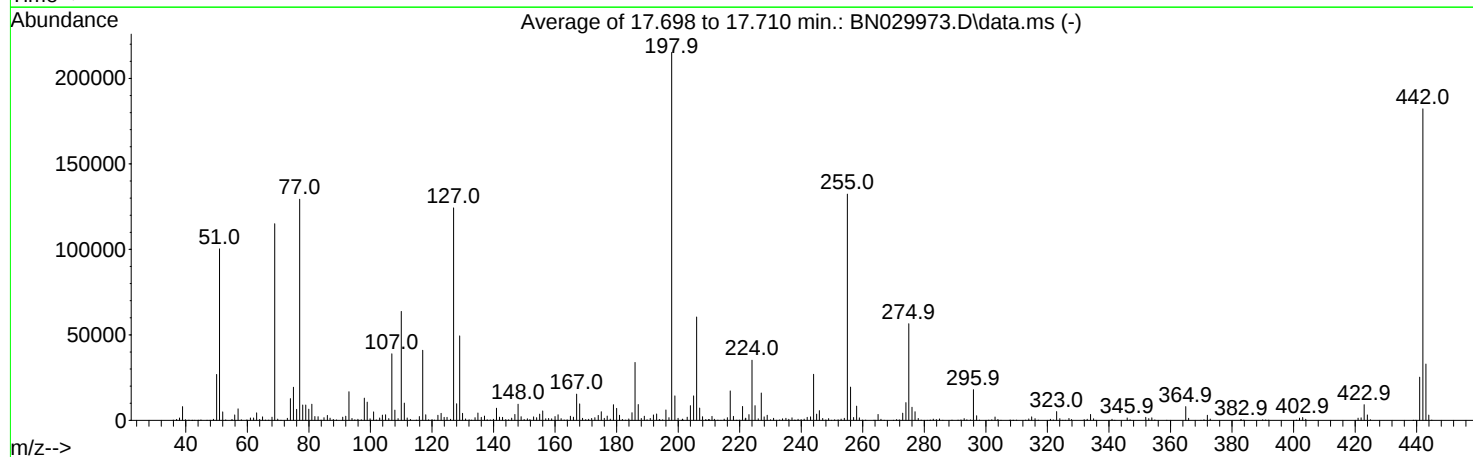


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022324\
Data File : BN029973.D
Acq On : 24 Feb 2024 02:16
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN012924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Feb 26 02:39:45 2024

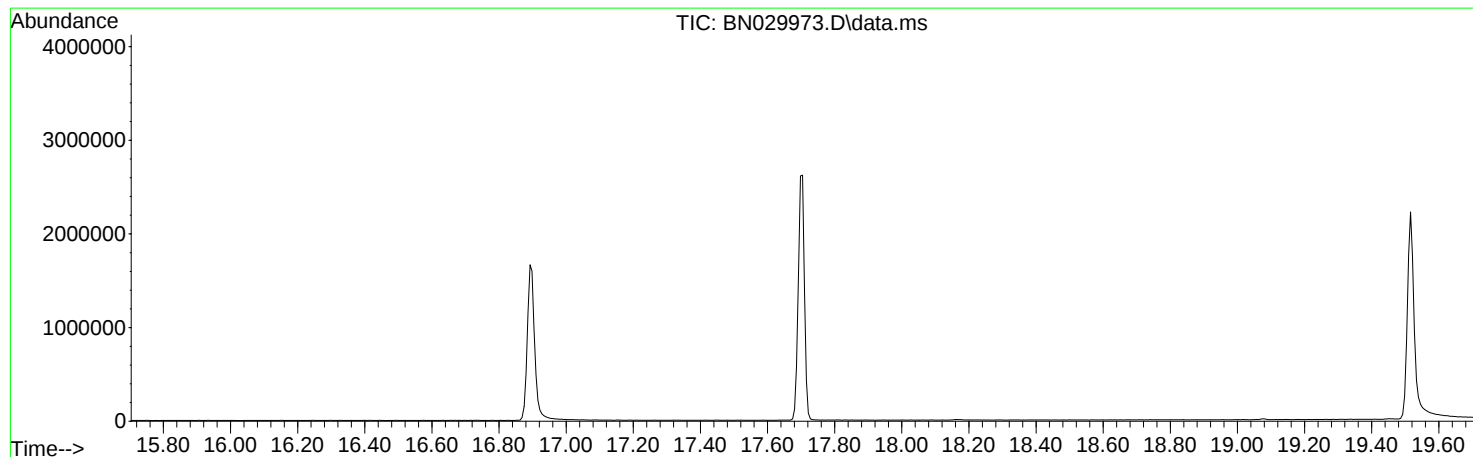




AutoFind: Scans 2484, 2485, 2486; Background Corrected with Scan 2476

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	46.7	100371	PASS
68	69	0.00	2	1.6	1885	PASS
69	198	0.00	100	53.5	115030	PASS
70	69	0.00	2	0.7	778	PASS
127	198	10	80	57.8	124283	PASS
197	198	0.00	2	0.7	1606	PASS
198	198	100	100	100.0	215147	PASS
199	198	5	9	6.7	14347	PASS
275	198	10	60	26.3	56520	PASS
365	198	1	100	3.8	8075	PASS
441	198	0.01	100	11.7	25235	PASS
442	442	50	100	100.0	182208	PASS
443	442	15	24	18.1	32920	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022324\
Data File : BN029973.D
Acq On : 24 Feb 2024 02:16
Operator : MA/JU
Sample : DFTTP
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTTP

Quant Time: Feb 24 05:21:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 24 05:20:21 2024
Response via : Initial Calibration

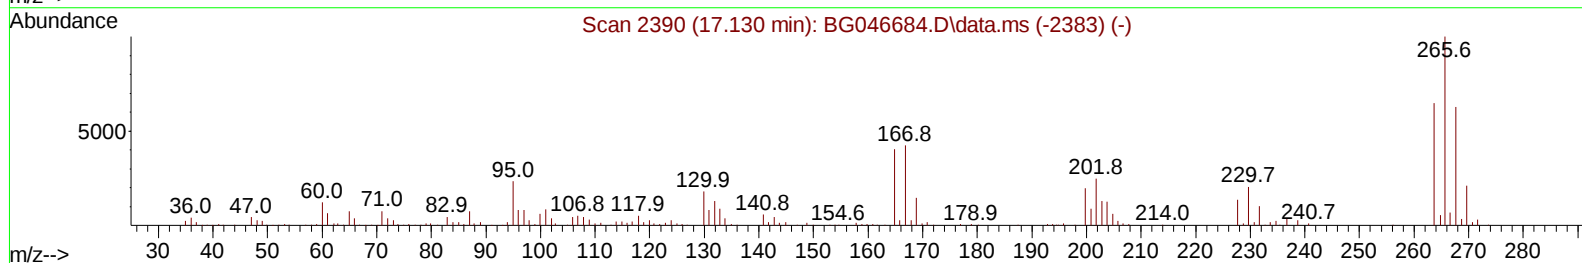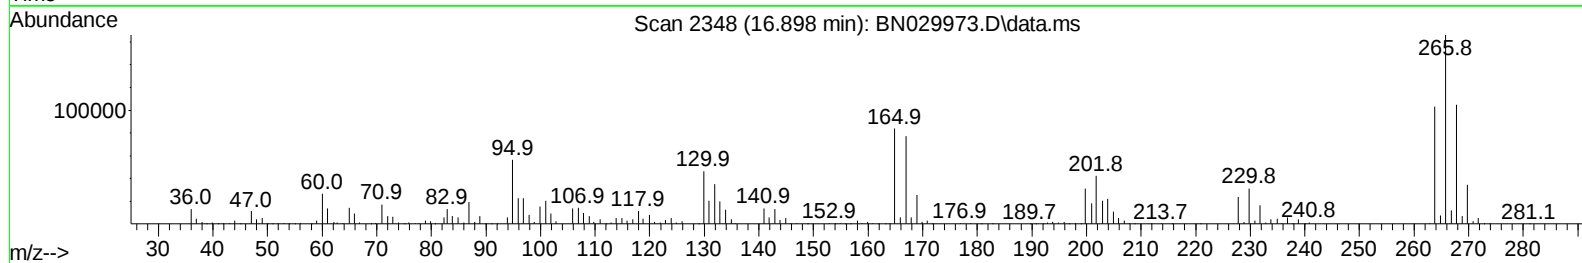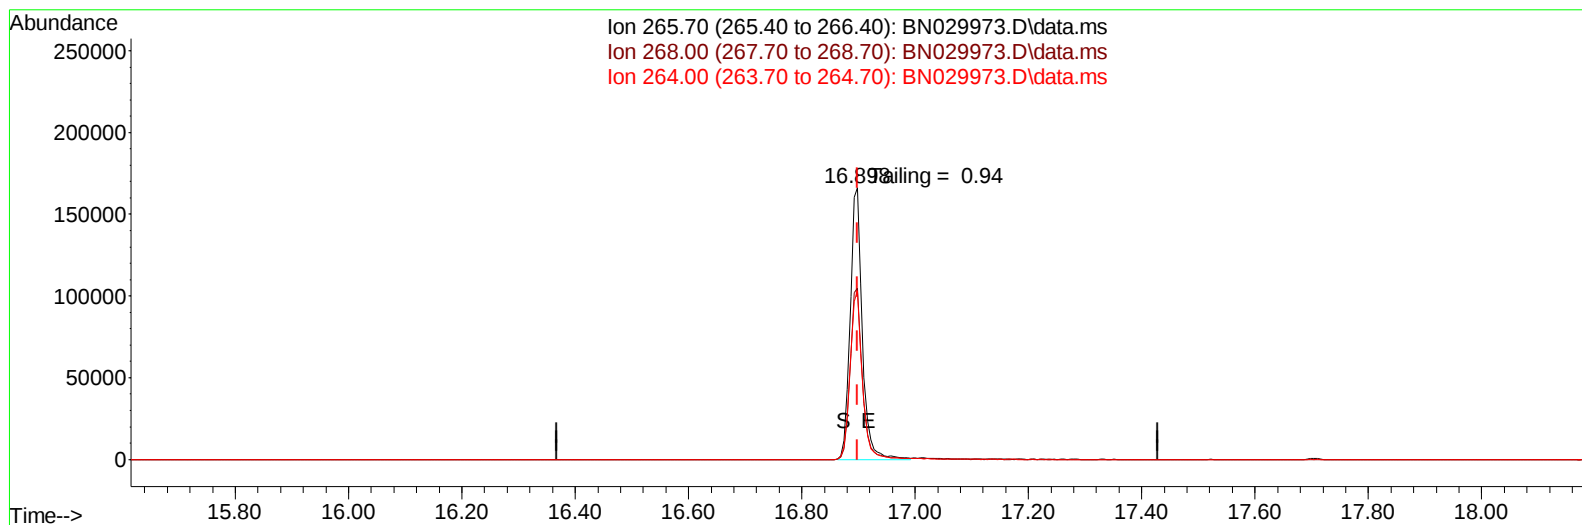

TIC: BN029973.D\data.ms

(70) Pentachlorophenol (C)

16.898min (0.000) 18620.64 ng




response 249298

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.15
264.00	61.60	62.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022324\
Data File : BN029973.D
Acq On : 24 Feb 2024 02:16
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Feb 24 05:21:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 24 05:20:21 2024
Response via : Initial Calibration

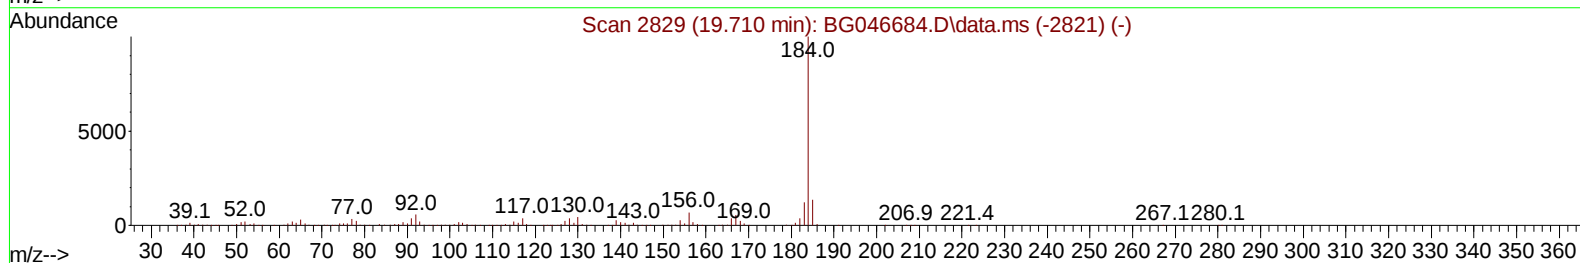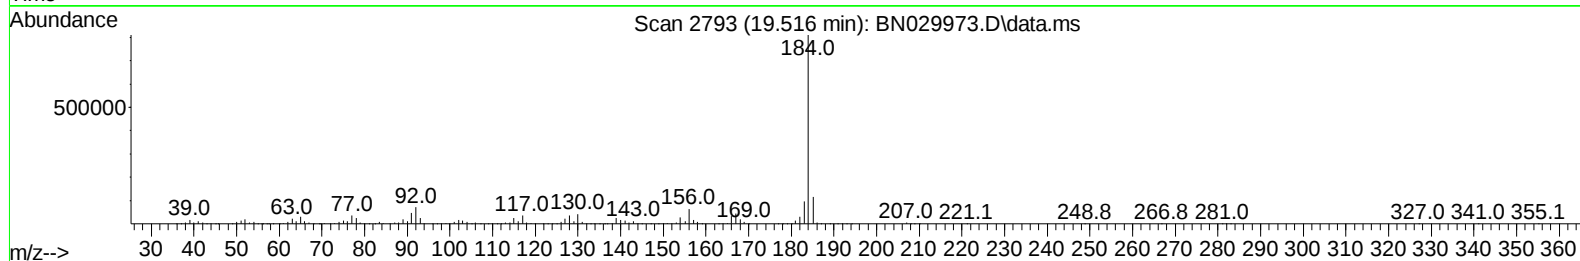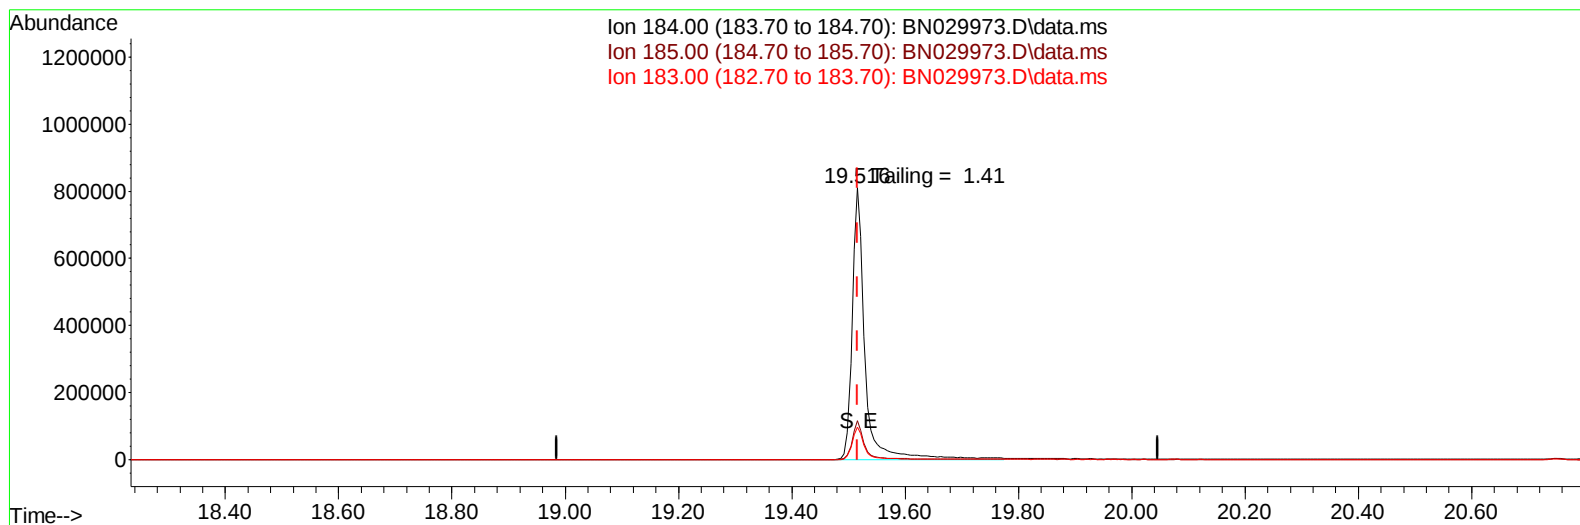

TIC: BN029973.D\data.ms

(77) Benzidine

19.516min (0.000) 0.00 ng

response 1258952

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.18
183.00	13.20	11.97
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/23/2024	BNA_N	<u>BN029973.D</u>
Compound Name	Response	Retention Time
DDT	733778	20.751
DDD	14345	20.31
DDE	480	19.792
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14825	748603	1.98

Instrument :
BNA_N
ClientSampleId :
DFTPP