
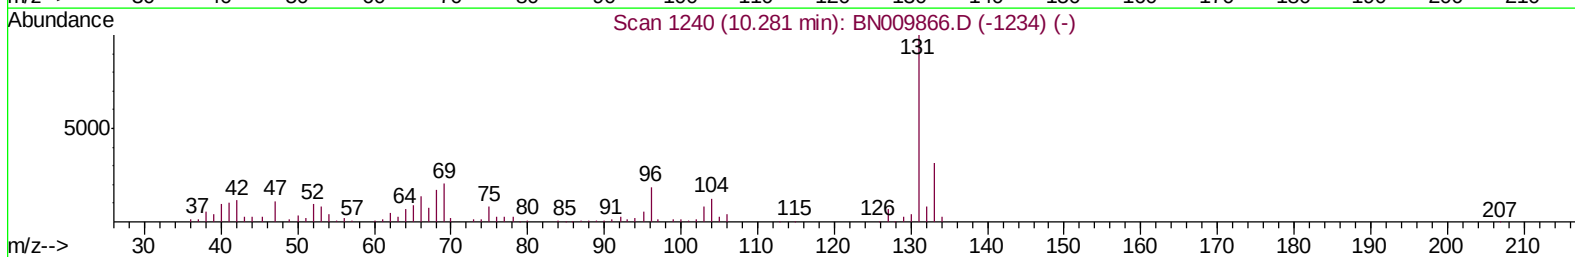
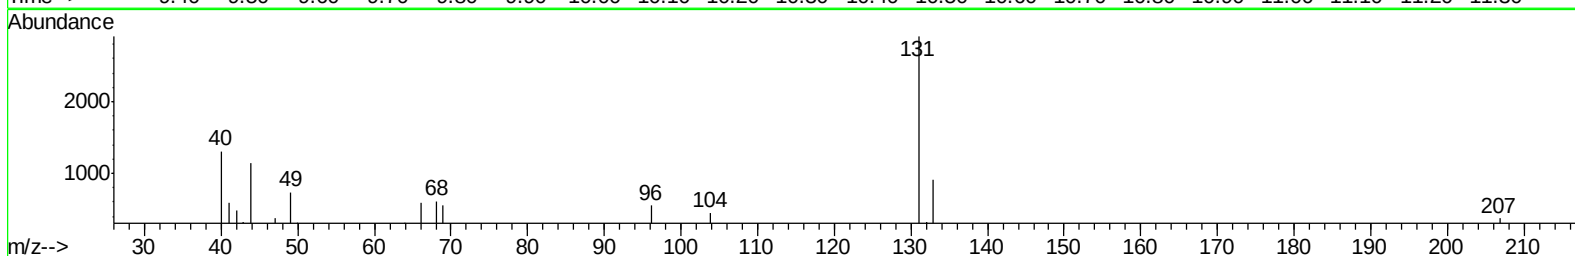


Data File : BN009871.D  
Acq On : 24 Feb 2020 19:51  
Operator : CG/JU  
Sample : L1582-11  
Misc :  
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Feb 25 02:42:09 2020  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\SOM-EPA-BN021220MA.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Tue Feb 25 02:39:29 2020  
Response via : Initial Calibration

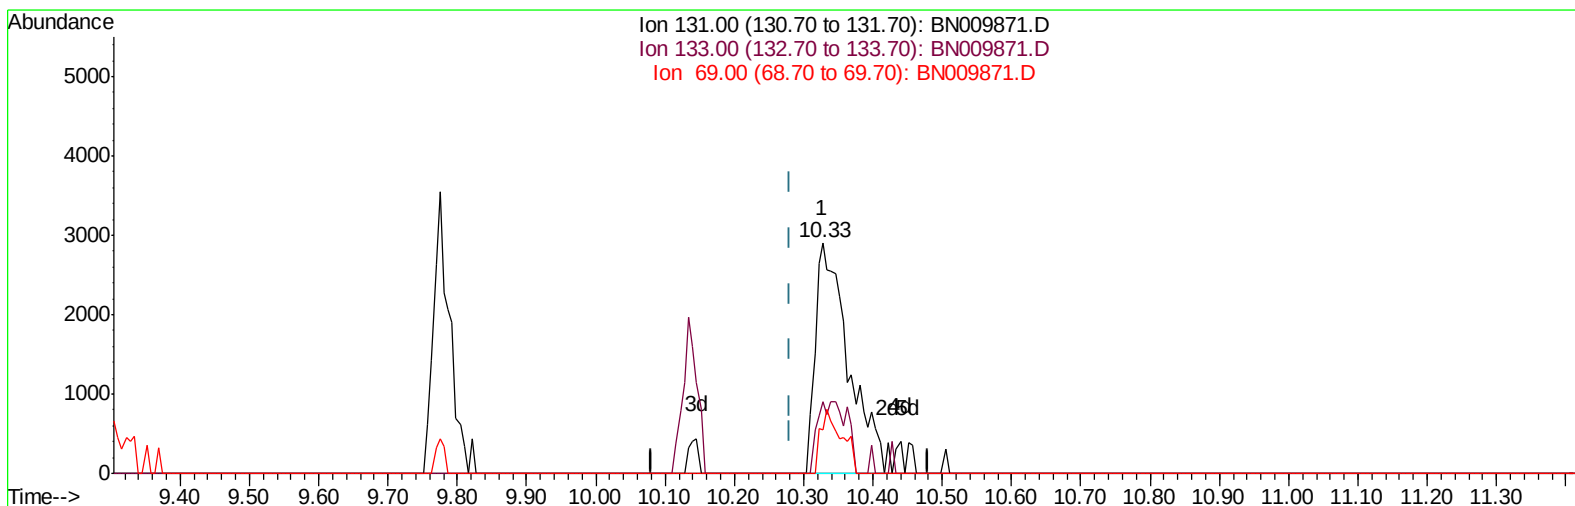

TIC: BN009871.D

(29) 4-Chloroaniline-d4 (S)

10.328min (+0.047) 1.38ng/ul m

response 9553

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 131.00 | 100   | 100   |
| 133.00 | 33.00 | 31.07 |
| 69.00  | 22.10 | 18.80 |
| 0.00   | 0.00  | 0.00  |