
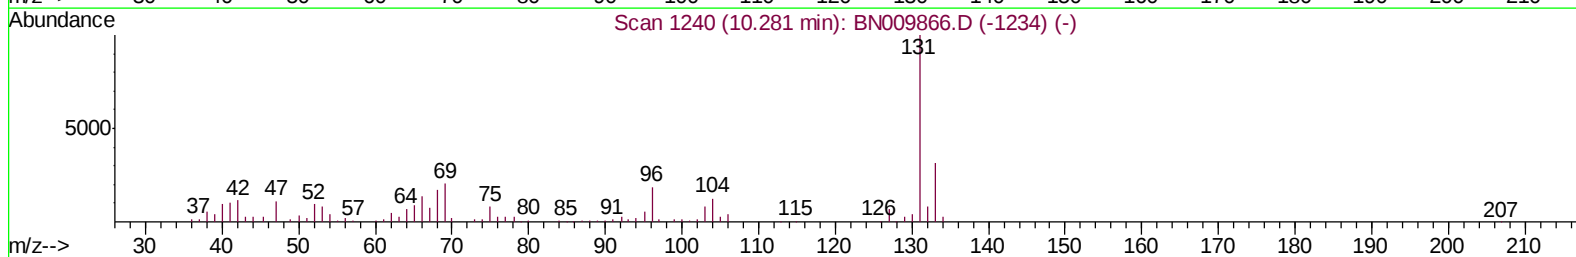
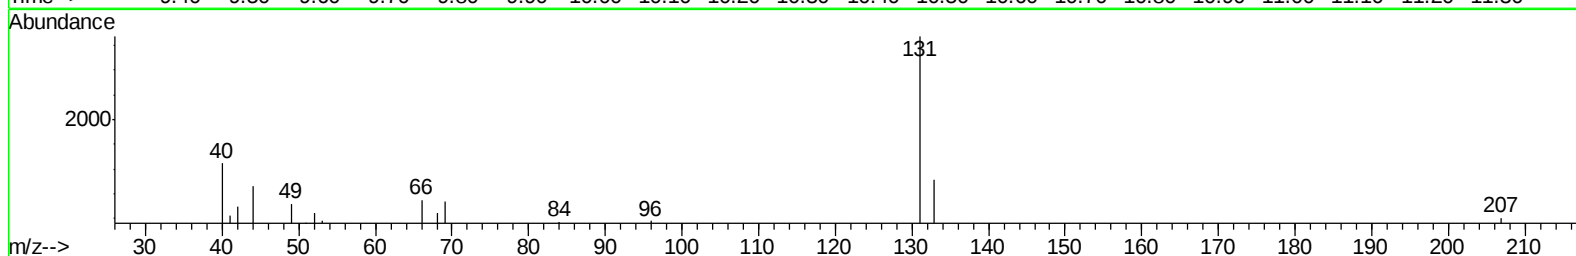


Data File : BN009872.D
Acq On : 24 Feb 2020 20:28
Operator : CG/JU
Sample : L1582-12
Misc :
ALS Vial : 11 Sample Multiplier: 1

Quant Time: Feb 25 02:42:16 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 25 02:39:29 2020
Response via : Initial Calibration

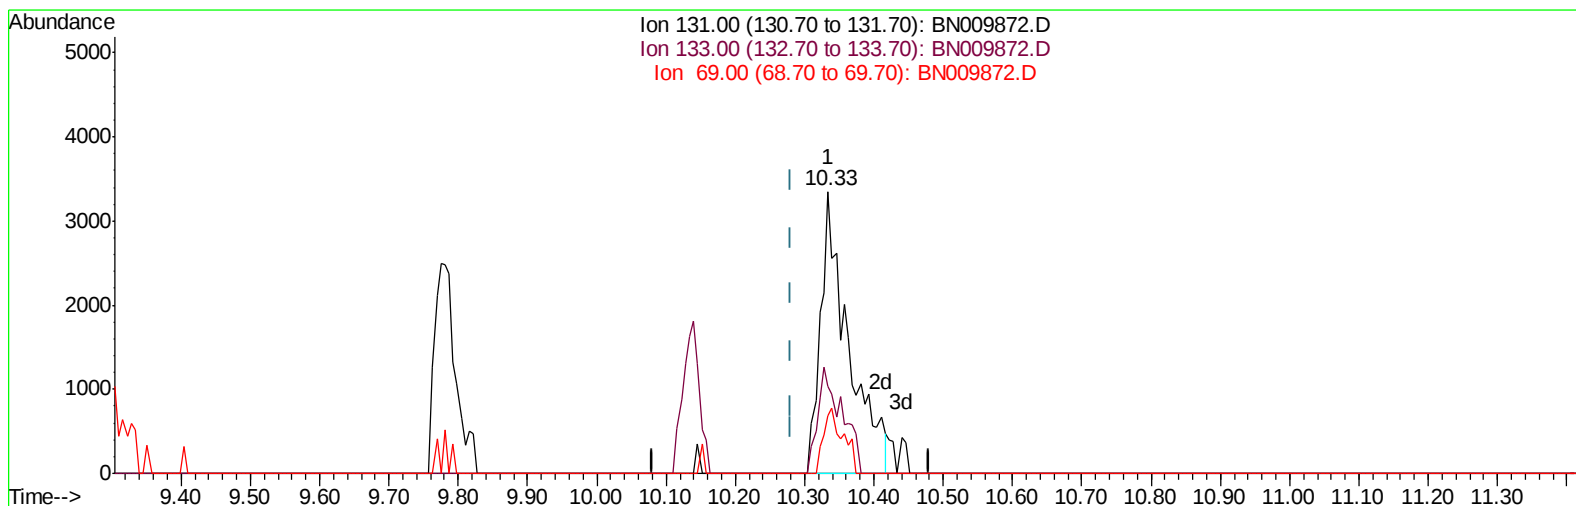

TIC: BN009872.D

(29) 4-Chloroaniline-d4 (S)

10.334min (+0.053) 1.46ng/ul m

response 9286

Ion	Exp%	Act%
131.00	100	100
133.00	33.00	30.76
69.00	22.10	20.31
0.00	0.00	0.00