
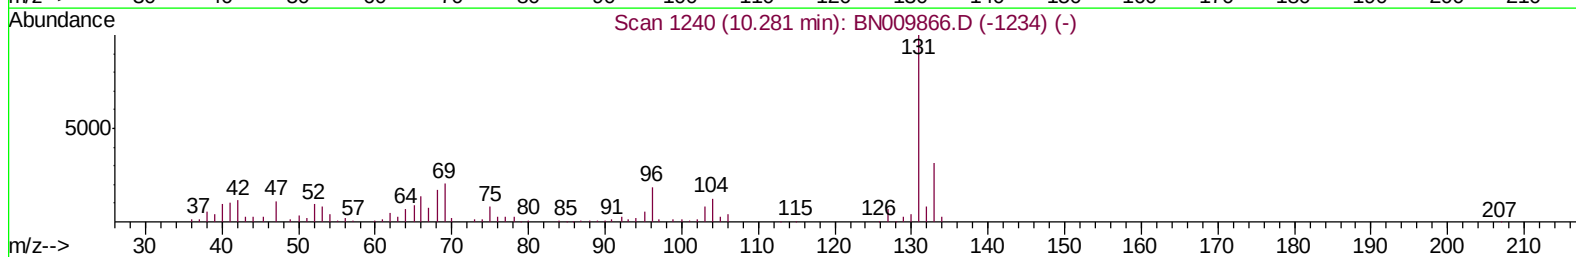
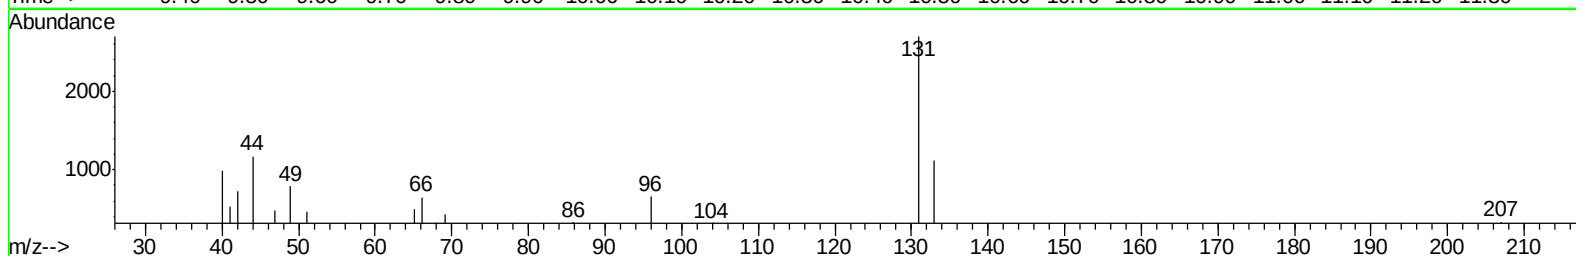


Data File : BN009874.D
Acq On : 24 Feb 2020 21:40
Operator : CG/JU
Sample : L1582-14
Misc :
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Feb 25 02:42:30 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 25 02:39:29 2020
Response via : Initial Calibration

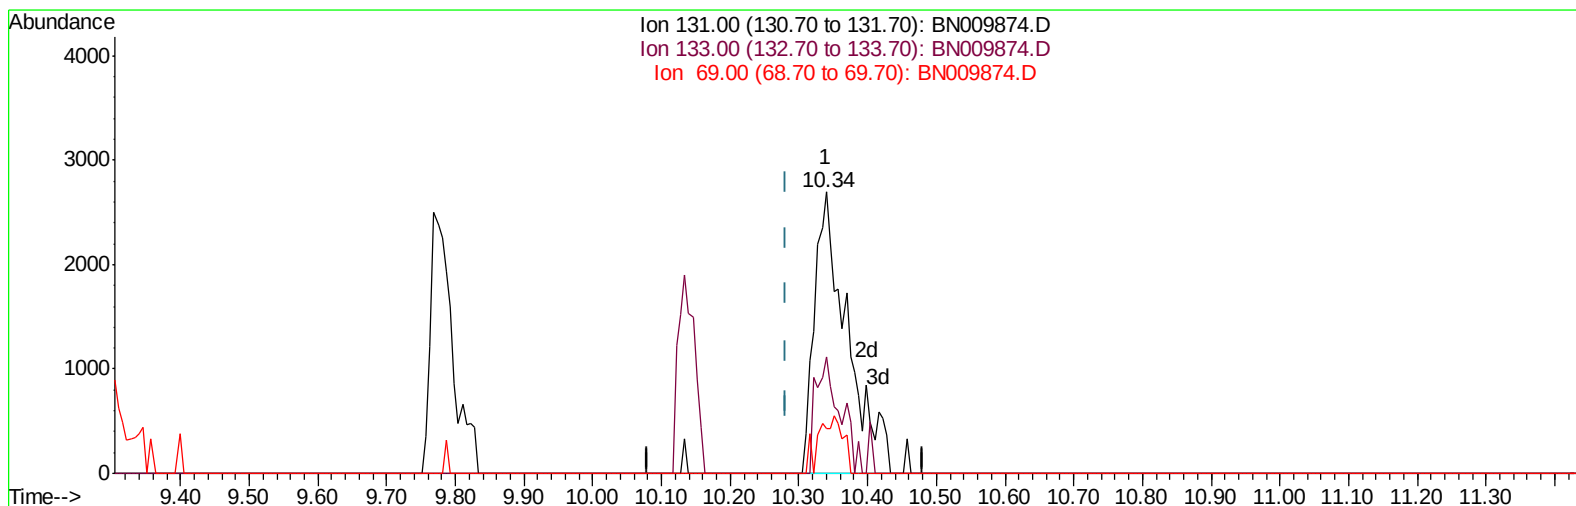

TIC: BN009874.D

(29) 4-Chloroaniline-d4 (S)

10.340min (+0.059) 1.25ng/ul m

response 8931

Ion	Exp%	Act%
131.00	100	100
133.00	33.00	41.22#
69.00	22.10	15.83#
0.00	0.00	0.00