
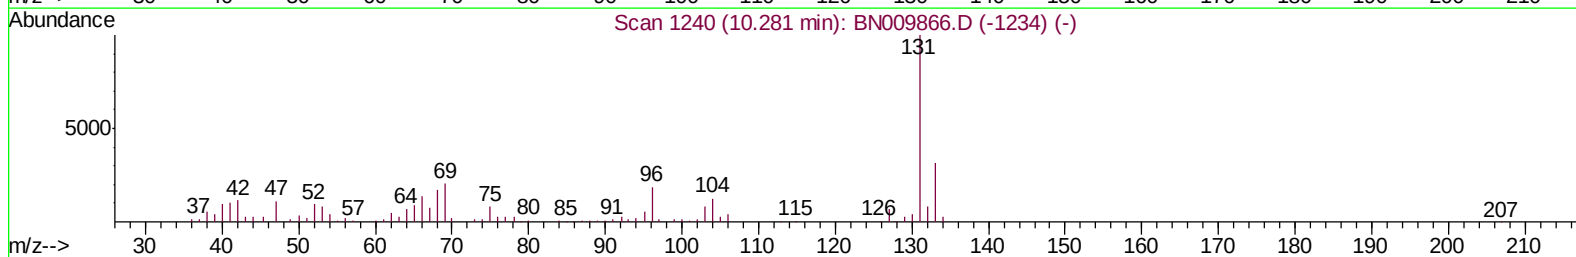
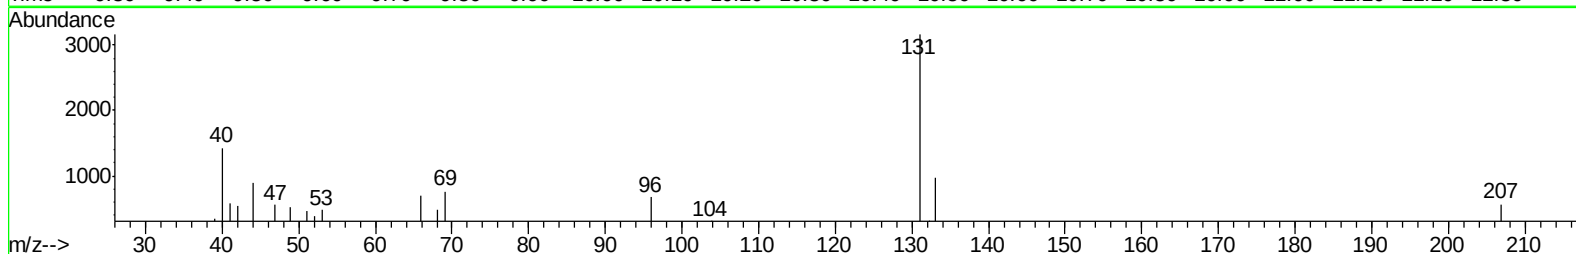


Data File : BN009875.D
Acq On : 24 Feb 2020 22:16
Operator : CG/JU
Sample : L1582-17
Misc :
ALS Vial : 14 Sample Multiplier: 1

Quant Time: Feb 25 02:42:36 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 25 02:39:29 2020
Response via : Initial Calibration

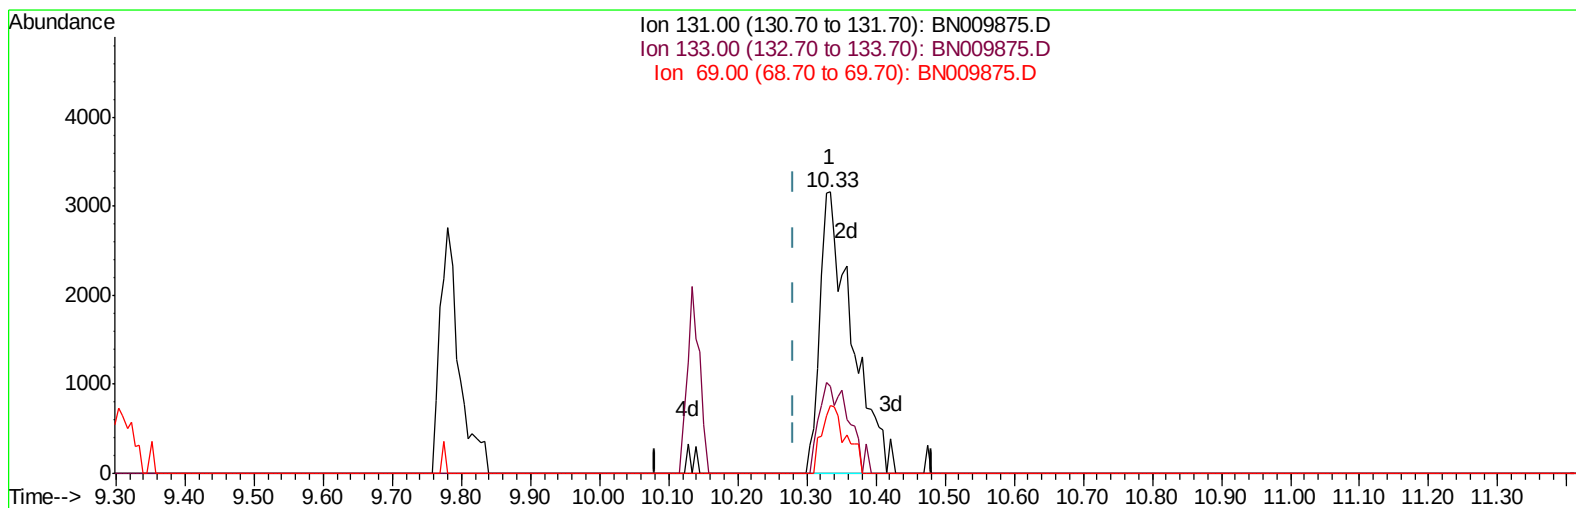

TIC: BN009875.D

(29) 4-Chloroaniline-d4 (S)

10.334min (+0.053) 1.58ng/ul m

response 9916

Ion	Exp%	Act%
131.00	100	100
133.00	33.00	30.95
69.00	22.10	24.15
0.00	0.00	0.00