
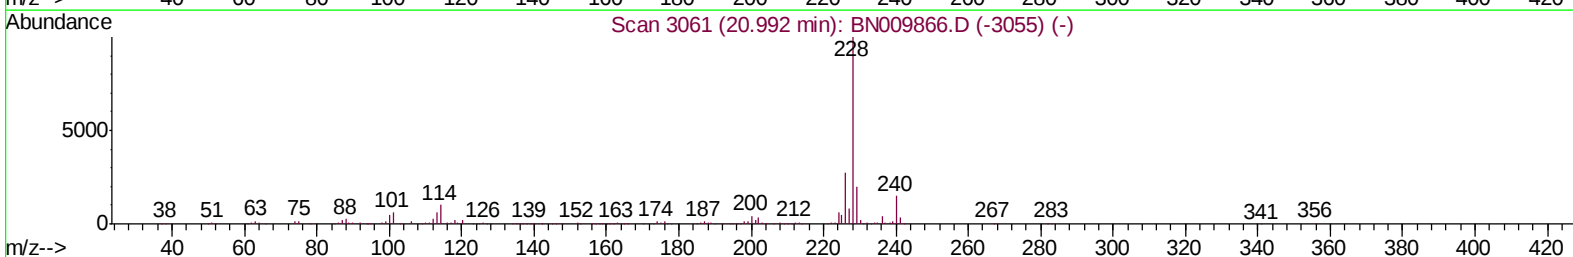
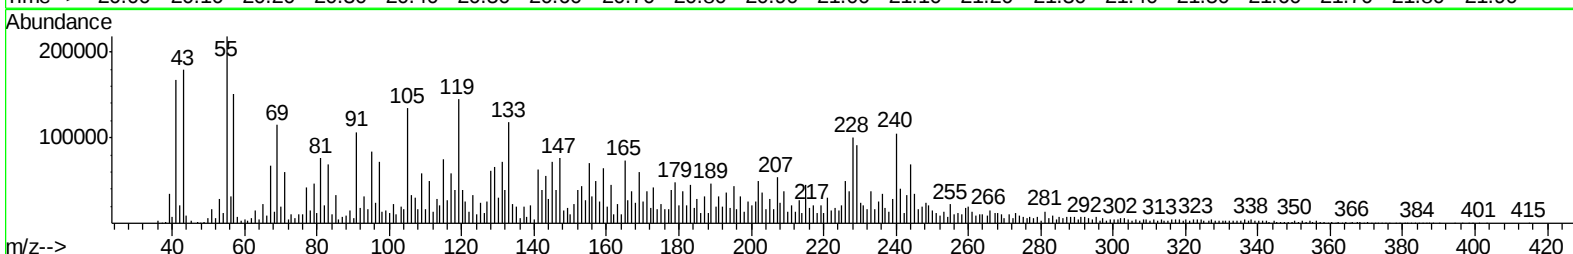


Data File : BN009881.D
Acq On : 25 Feb 2020 01:52
Operator : CG/JU
Sample : L1418-05
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Feb 25 03:38:23 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 25 02:39:29 2020
Response via : Initial Calibration

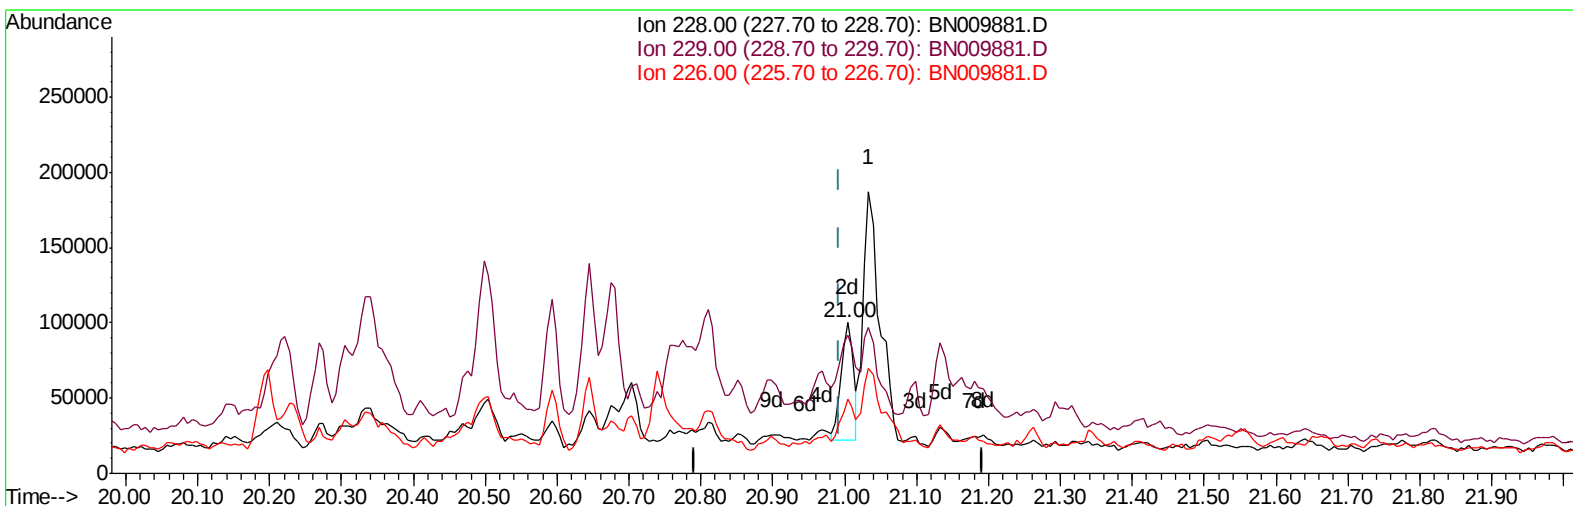

TIC: BN009881.D

(83) Benzo(a)anthracene

21.004min (+0.012) 2.38ng/ul m

response 96479

Ion	Exp%	Act%
228.00	100	100
229.00	18.70	91.59#
226.00	26.80	49.57#
0.00	0.00	0.00