
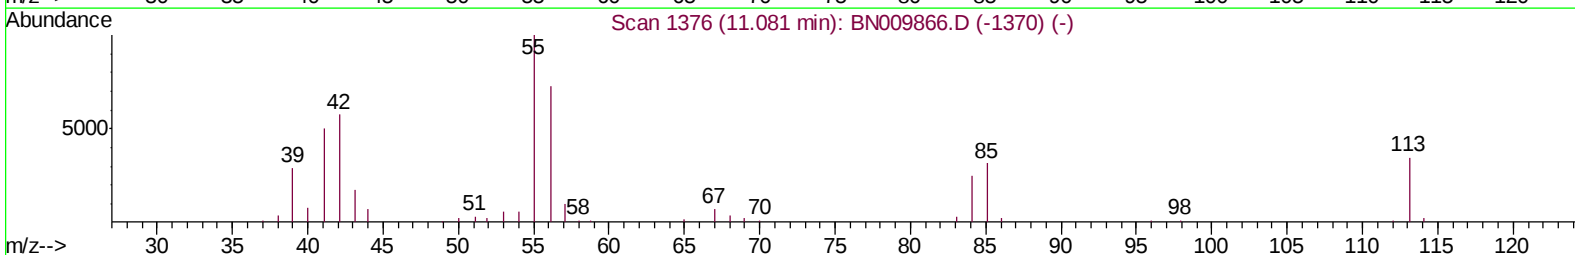
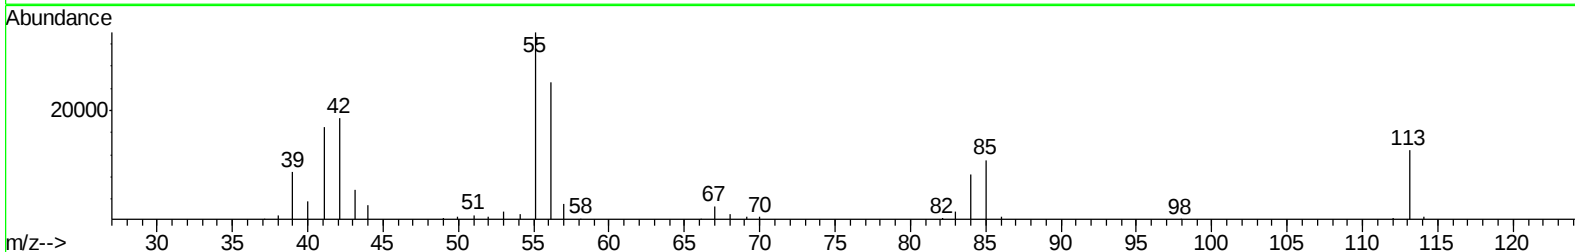


Data File : BN009883.D
Acq On : 25 Feb 2020 04:16
Operator : CG/JU
Sample : SSTDCCC020
Misc :
ALS Vial : 37 Sample Multiplier: 1

Quant Time: Feb 25 04:54:04 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 25 02:39:29 2020
Response via : Initial Calibration

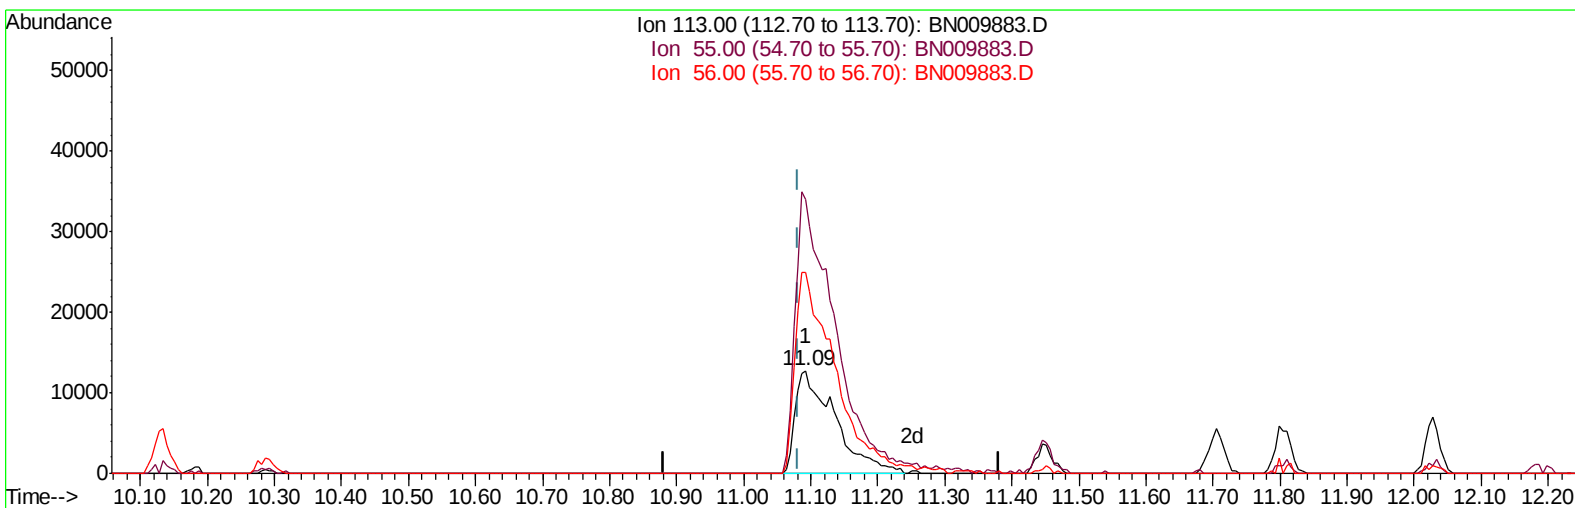

TIC: BN009883.D

(32) Caprolactam

11.093min (+0.012) 21.13ng/ul m

response 52189

Ion	Exp%	Act%
113.00	100	100
55.00	261.40	266.77
56.00	202.00	195.90
0.00	0.00	0.00