
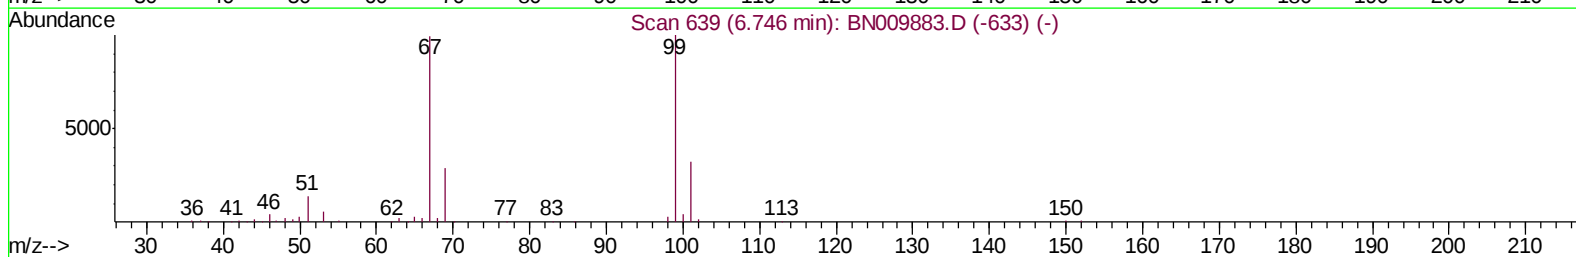
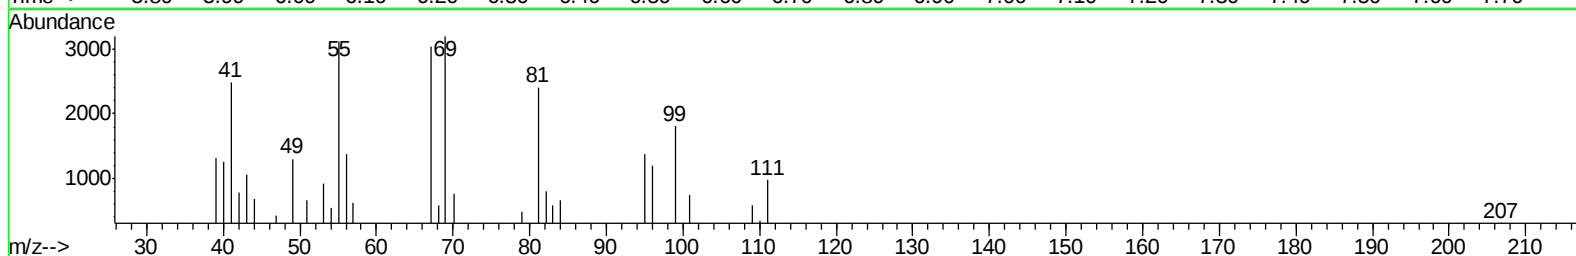


Data File : BN009887.D
Acq On : 25 Feb 2020 06:41
Operator : CG/JU
Sample : L1418-16DL 30X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Quant Time: Feb 25 07:25:00 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 25 07:22:29 2020
Response via : Initial Calibration

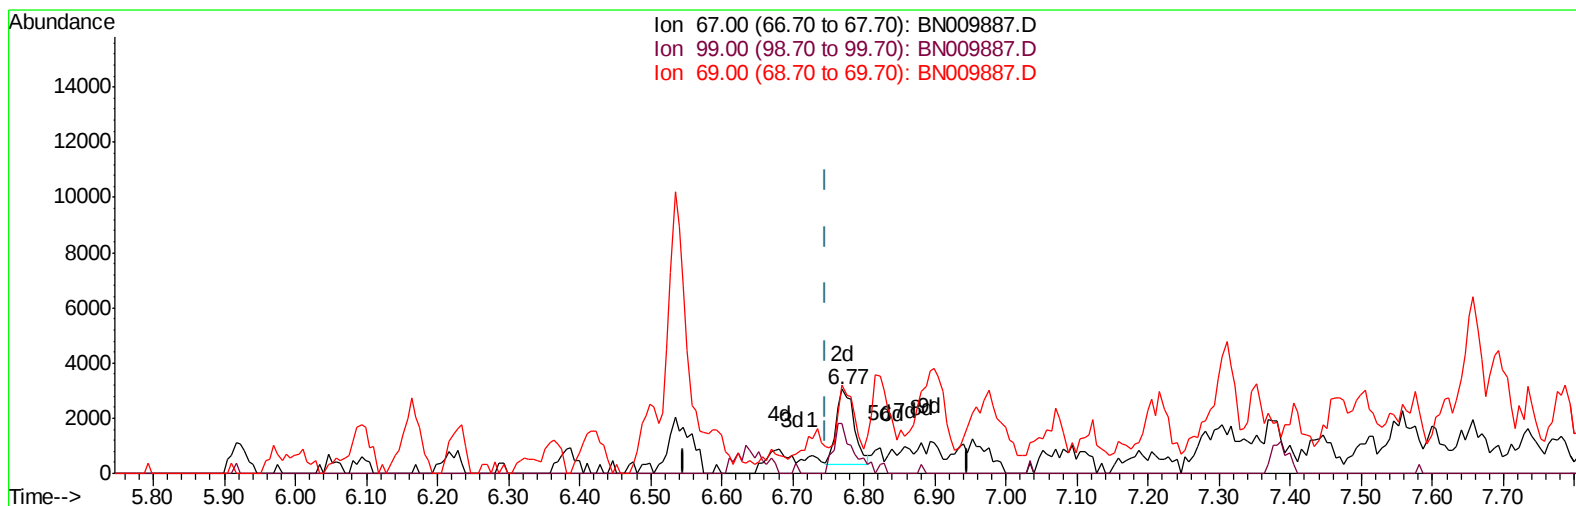

TIC: BN009887.D

(7) Bis-(2-Chloroethyl)ether-d8 (S)

6.769min (+0.024) 0.91ng/ul m

response 4687

Ion	Exp%	Act%
67.00	100	100
99.00	106.90	59.37#
69.00	28.30	105.16#
0.00	0.00	0.00