
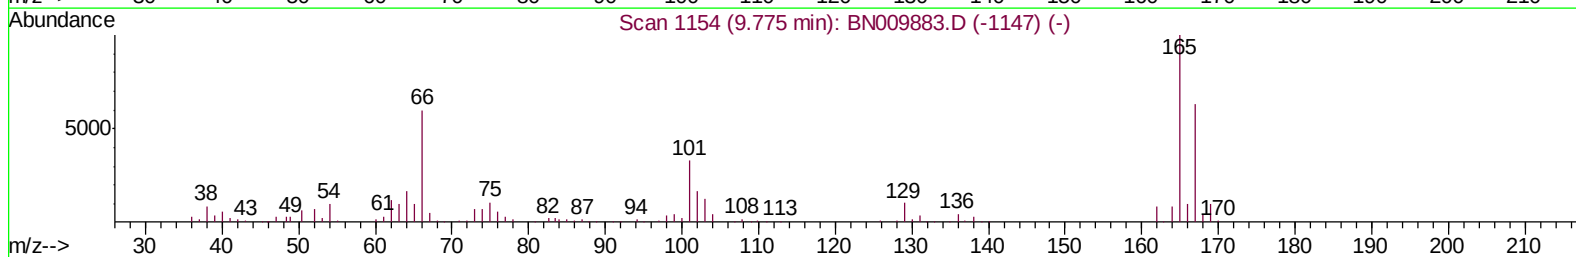
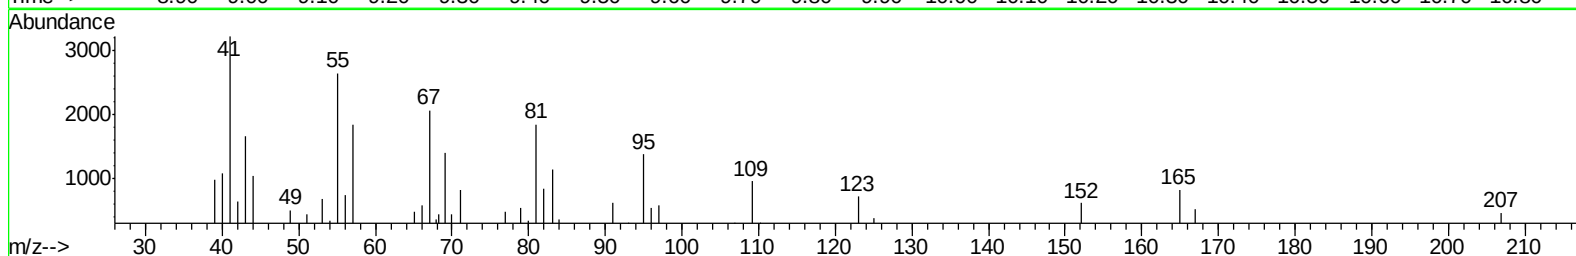


Data File : BN009887.D
Acq On : 25 Feb 2020 06:41
Operator : CG/JU
Sample : L1418-16DL 30X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Quant Time: Feb 25 07:25:00 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 25 07:22:29 2020
Response via : Initial Calibration

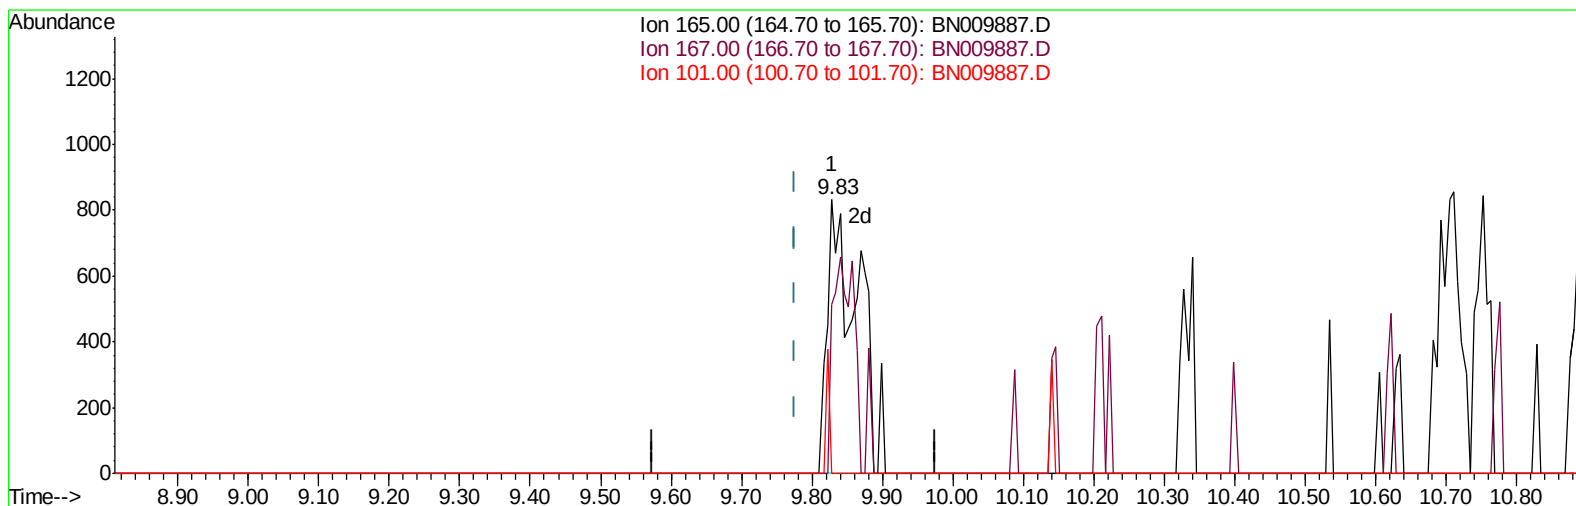

TIC: BN009887.D

(26) 2,4-Dichlorophenol-d3 (S)

9.828min (+0.053) 0.41ng/ul m

response 2392

Ion	Exp%	Act%
165.00	100	100
167.00	64.20	61.90
101.00	36.10	0.00#
0.00	0.00	0.00