
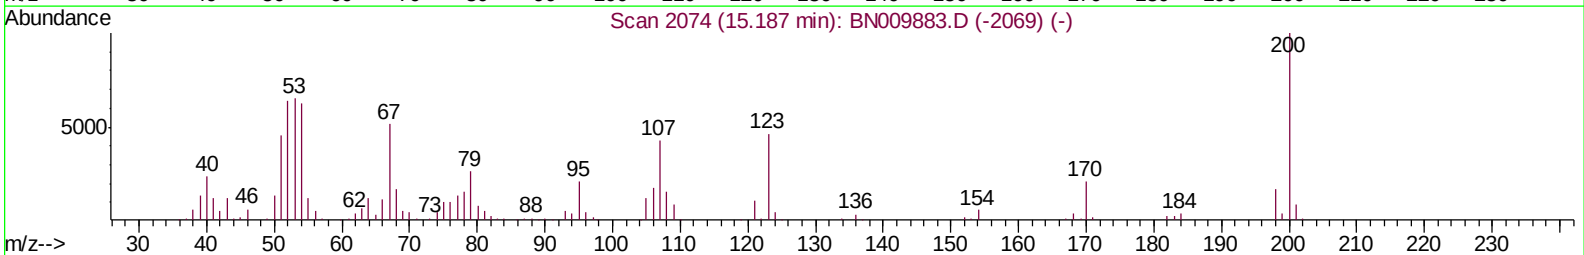
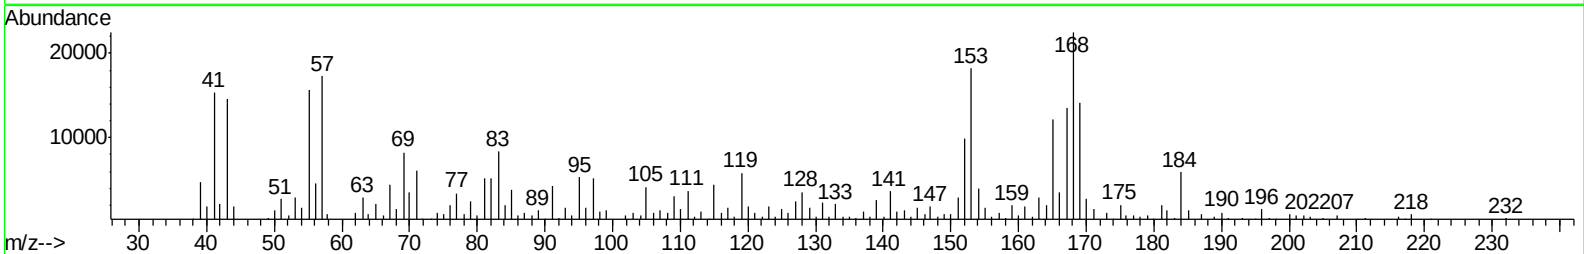


Data File : BN009887.D
Acq On : 25 Feb 2020 06:41
Operator : CG/JU
Sample : L1418-16DL 30X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Quant Time: Feb 25 07:25:00 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 25 07:22:29 2020
Response via : Initial Calibration

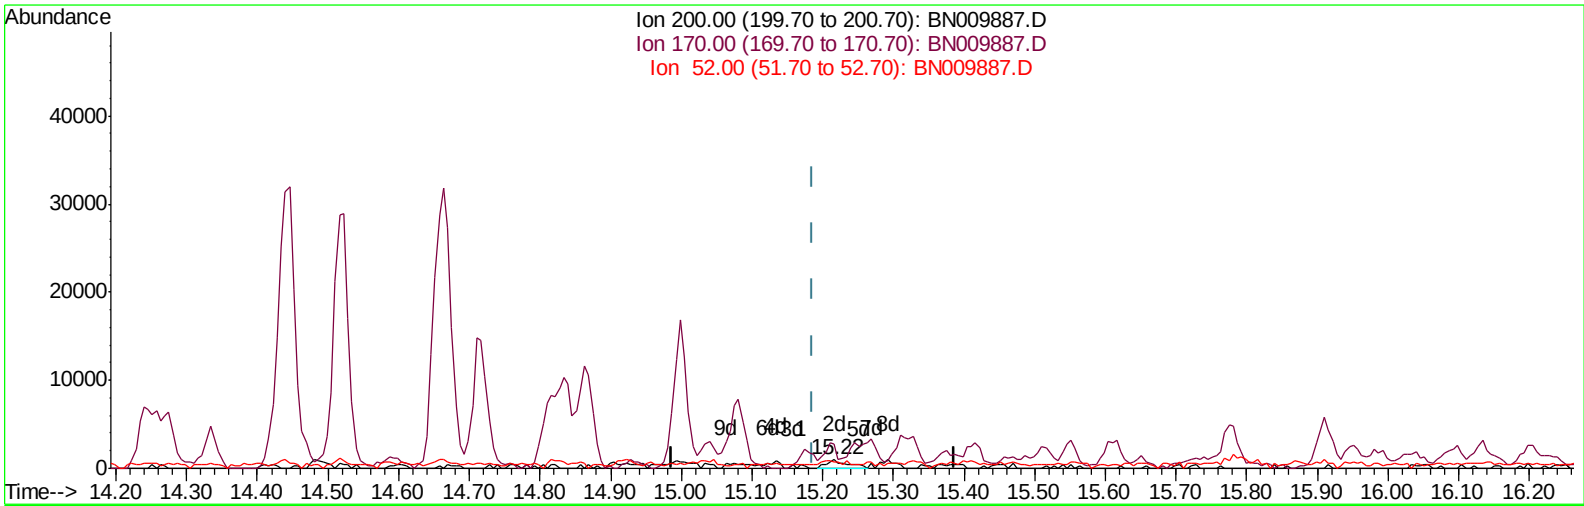

TIC: BN009887.D

(63) 4,6-Dinitro-2-methylphenol-d2 (S)

15.216min (+0.029) 0.67ng/ul m

response 2066

Ion	Exp%	Act%
200.00	100	100
170.00	22.10	293.59#
52.00	71.30	81.49
0.00	0.00	0.00