
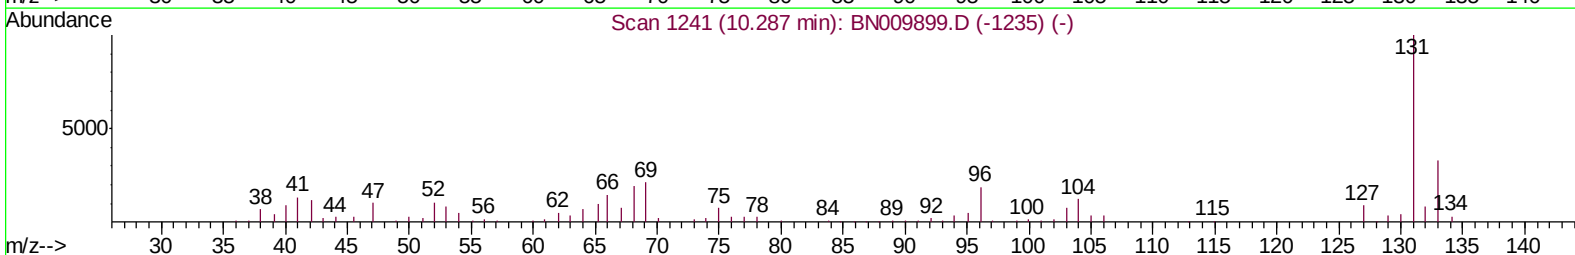
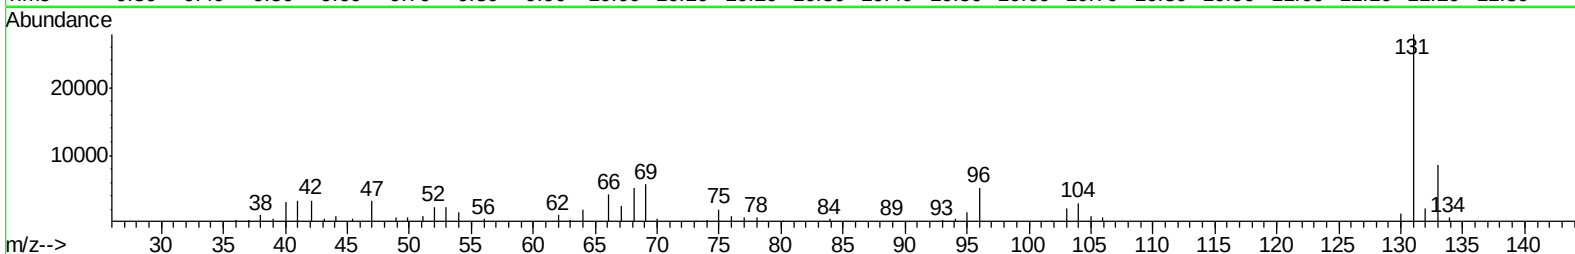


Data File : BN009902.D
Acq On : 25 Feb 2020 15:41
Operator : CG/JU
Sample : L1418-04
Misc :
ALS Vial : 40 Sample Multiplier: 1

Quant Time: Feb 26 07:09:59 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 26 07:04:59 2020
Response via : Initial Calibration

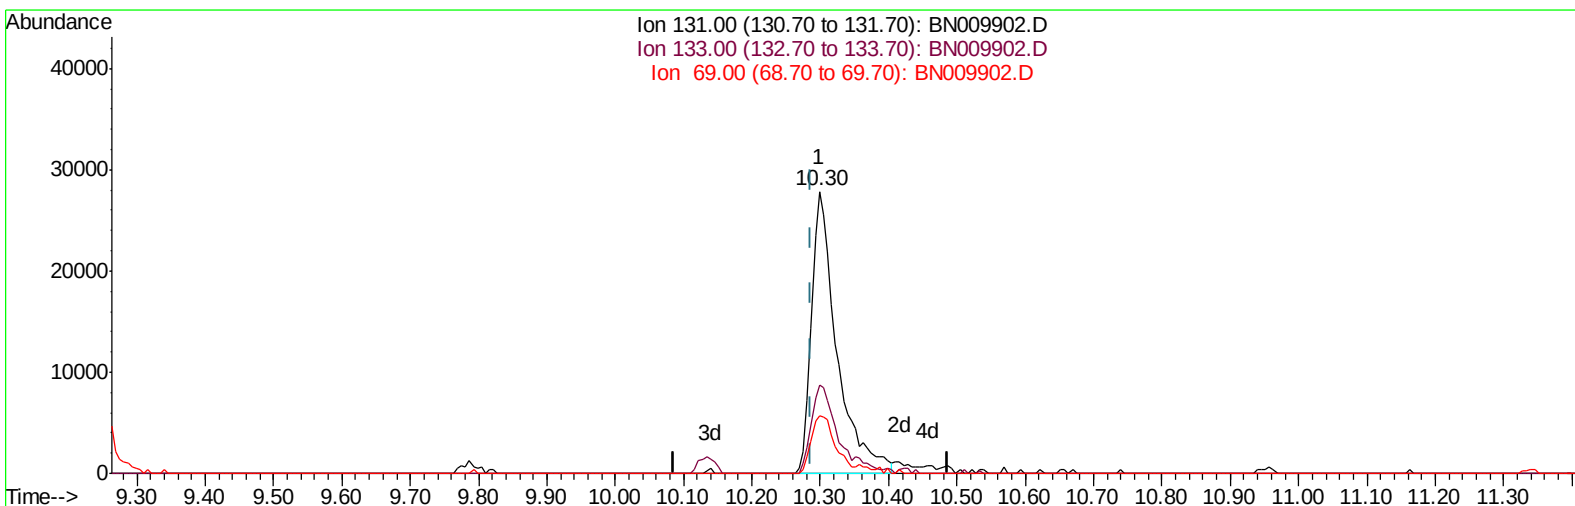

TIC: BN009902.D

(29) 4-Chloroaniline-d4 (S)
10.298min (+0.012) 11.26ng/ul m
response 71706

Ion	Exp%	Act%
131.00	100	100
133.00	33.00	31.25
69.00	22.10	20.45
0.00	0.00	0.00