
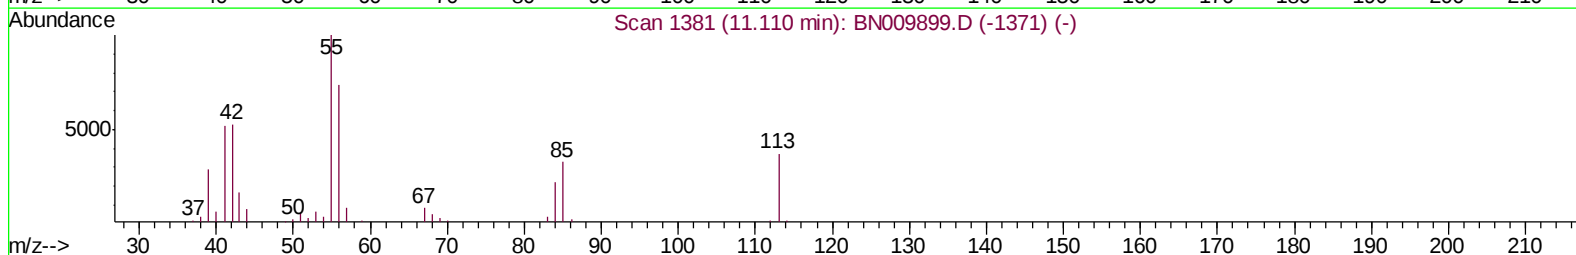
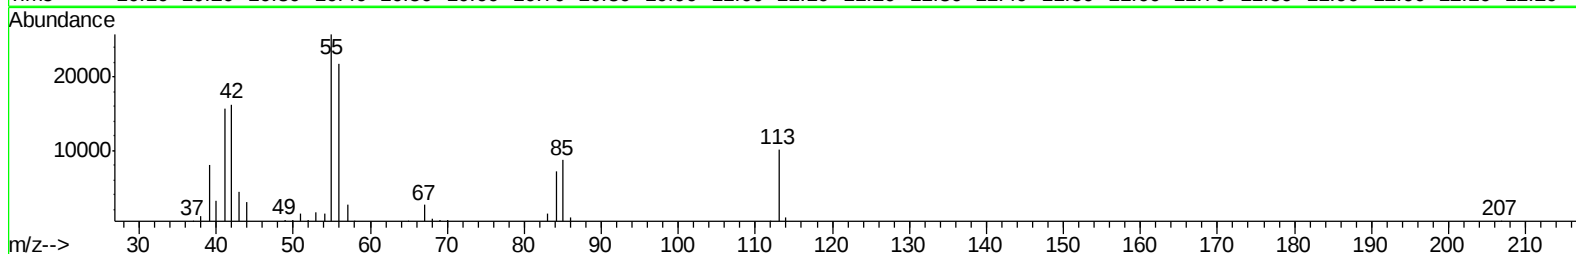


Data File : BN009913.D
Acq On : 25 Feb 2020 22:19
Operator : CG/JU
Sample : SSTDCCC020
Misc :
ALS Vial : 51 Sample Multiplier: 1

Quant Time: Feb 26 07:11:32 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 26 07:04:59 2020
Response via : Initial Calibration

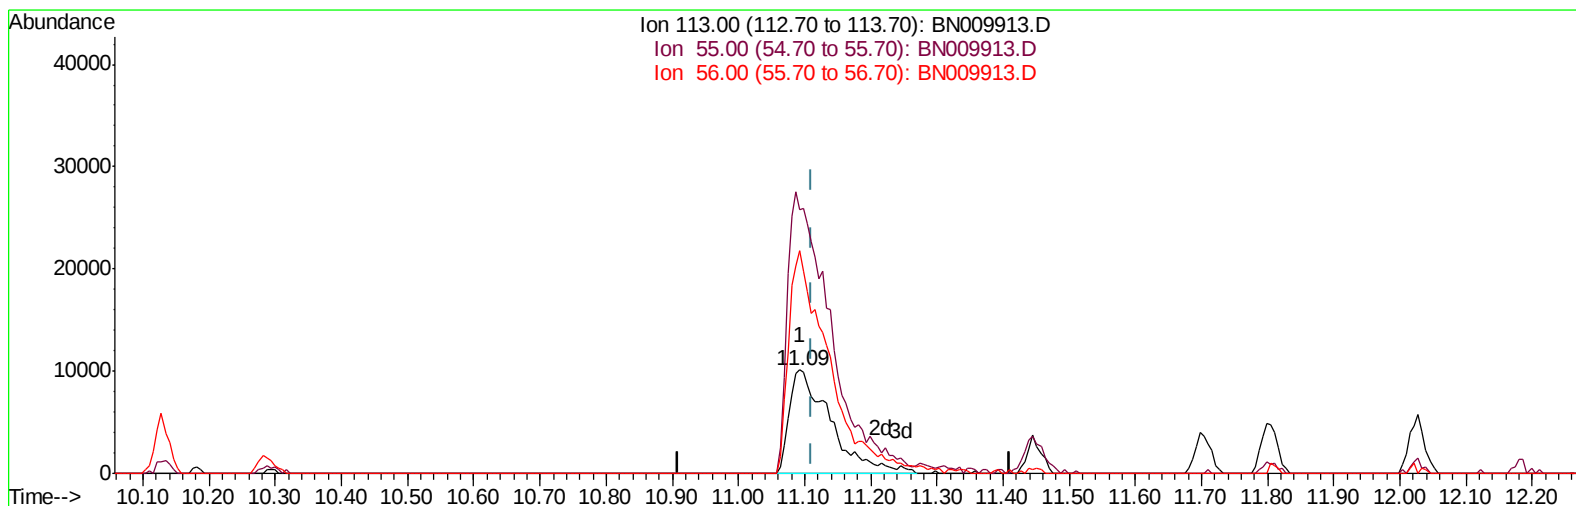

TIC: BN009913.D

(32) Caprolactam

11.092min (-0.018) 21.58ng/ul m

response 44107

Ion	Exp%	Act%
113.00	100	100
55.00	261.40	255.64
56.00	202.00	216.24
0.00	0.00	0.00