
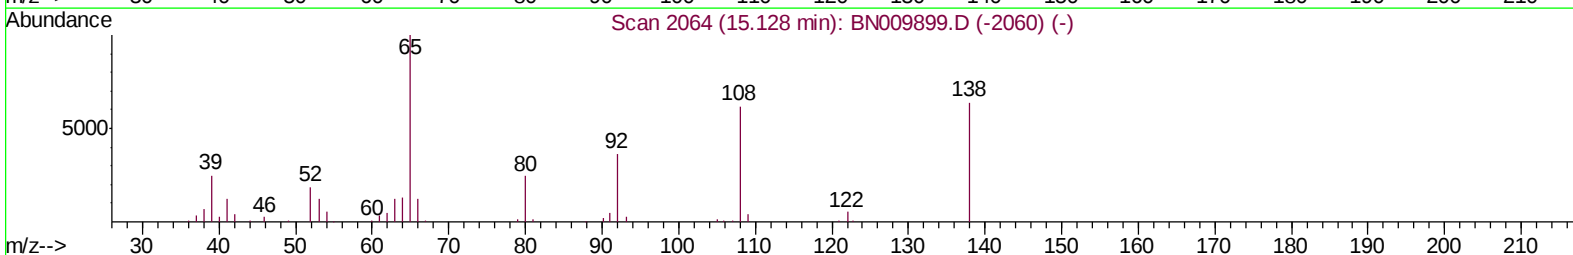
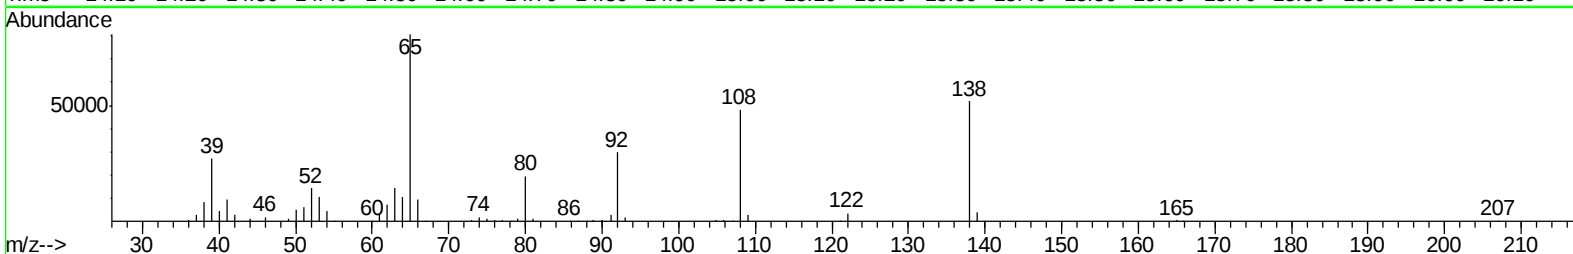


Data File : BN009913.D
Acq On : 25 Feb 2020 22:19
Operator : CG/JU
Sample : SSTDCCC020
Misc :
ALS Vial : 51 Sample Multiplier: 1

Quant Time: Feb 26 07:11:32 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 26 07:04:59 2020
Response via : Initial Calibration

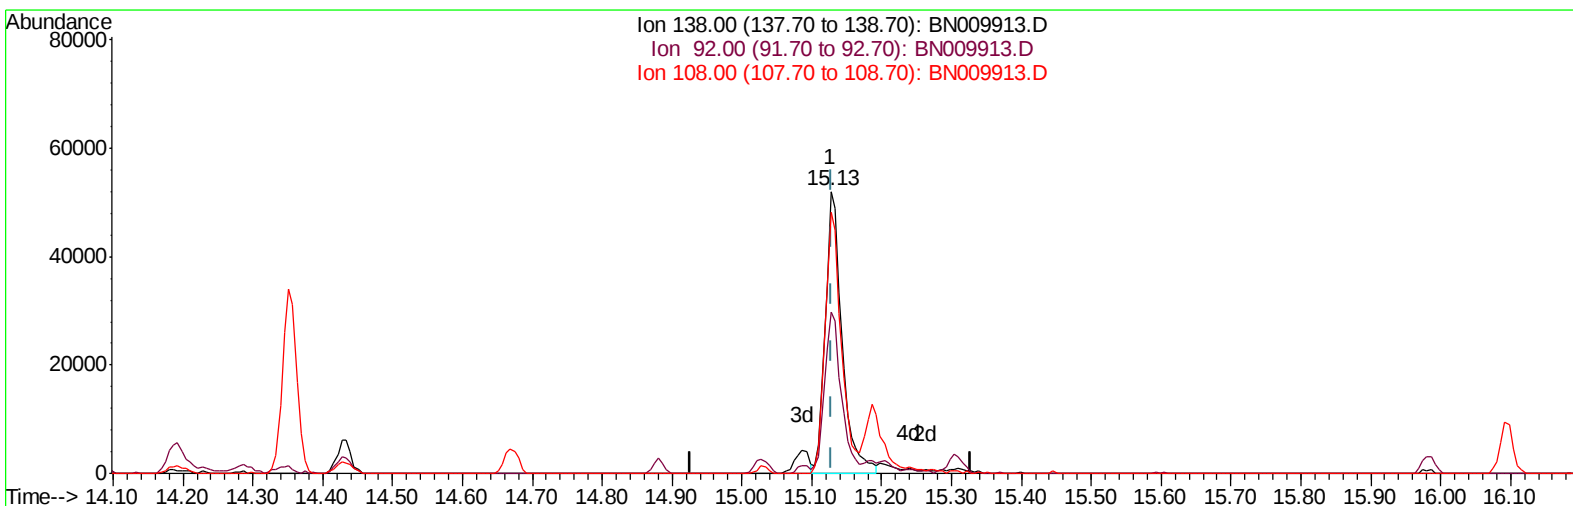

TIC: BN009913.D

(61) 4-Nitroaniline

15.128min (-0.000) 19.93ng/ul m

response 86692

Ion	Exp%	Act%
138.00	100	100
92.00	59.70	57.40
108.00	90.40	92.75
0.00	0.00	0.00