
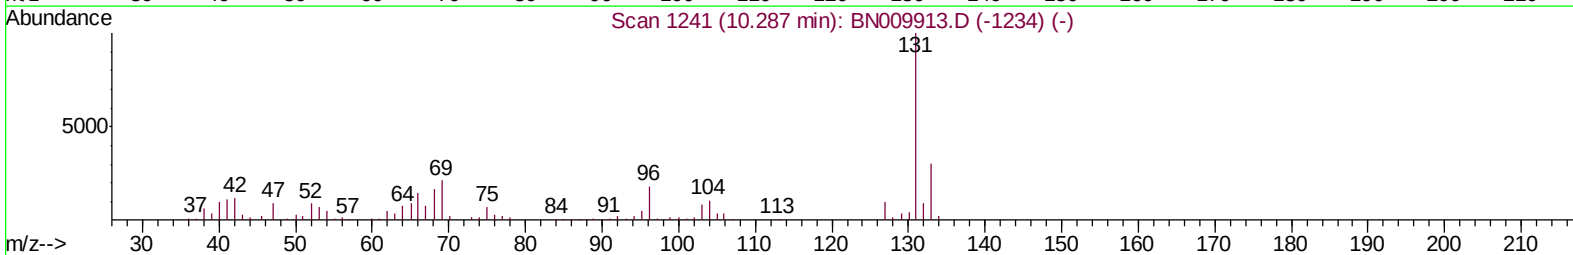
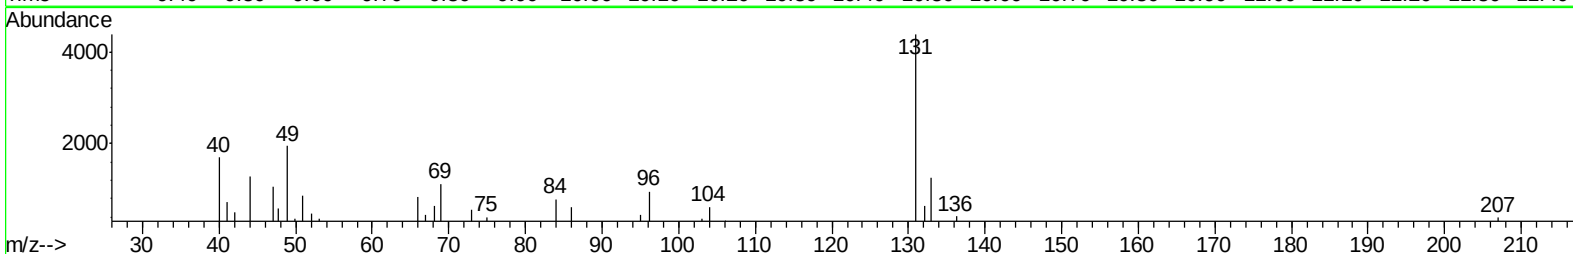


Data File : BN009918.D
Acq On : 26 Feb 2020 01:56
Operator : CG/JU
Sample : L1568-13
Misc :
ALS Vial : 56 Sample Multiplier: 1

Quant Time: Feb 26 07:58:46 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 26 07:56:07 2020
Response via : Initial Calibration

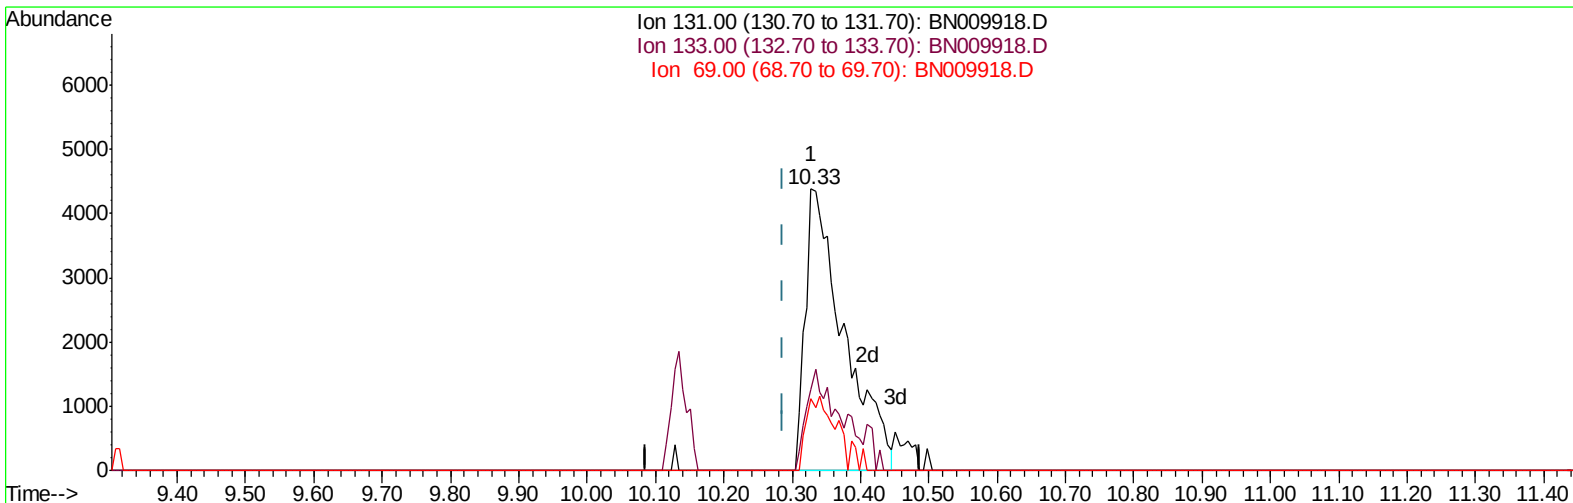

TIC: BN009918.D

(29) 4-Chloroaniline-d4 (S)

10.328min (+0.041) 2.64ng/ul m

response 17050

Ion	Exp%	Act%
131.00	100	100
133.00	33.00	28.80
69.00	22.10	25.56
0.00	0.00	0.00