
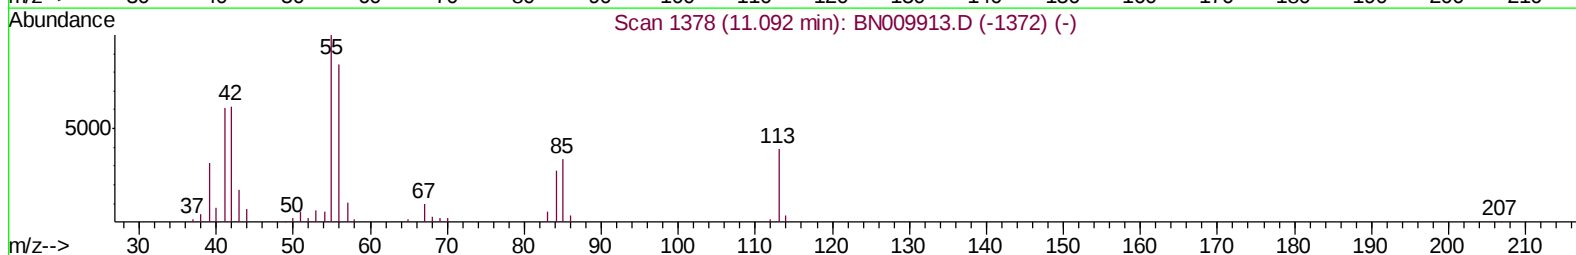
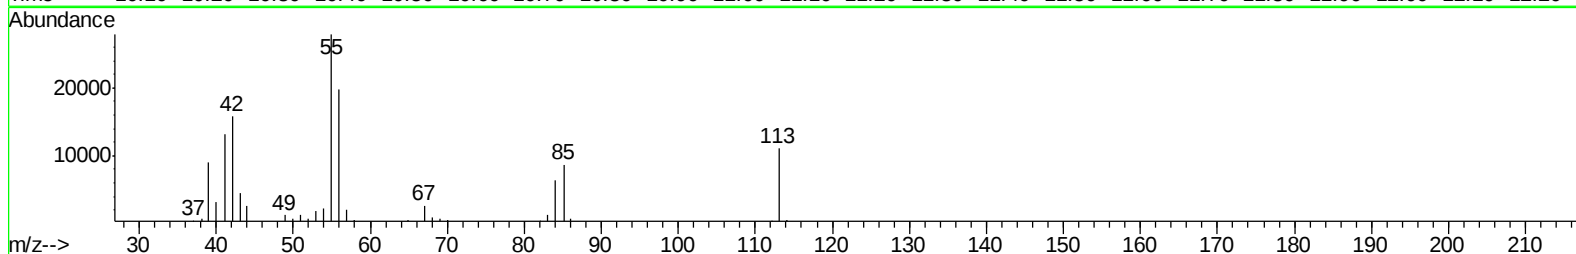


Data File : BN009919.D
Acq On : 26 Feb 2020 02:32
Operator : CG/JU
Sample : SSTDCCC020EC
Misc :
ALS Vial : 57 Sample Multiplier: 1

Quant Time: Feb 26 07:58:53 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 26 07:56:07 2020
Response via : Initial Calibration

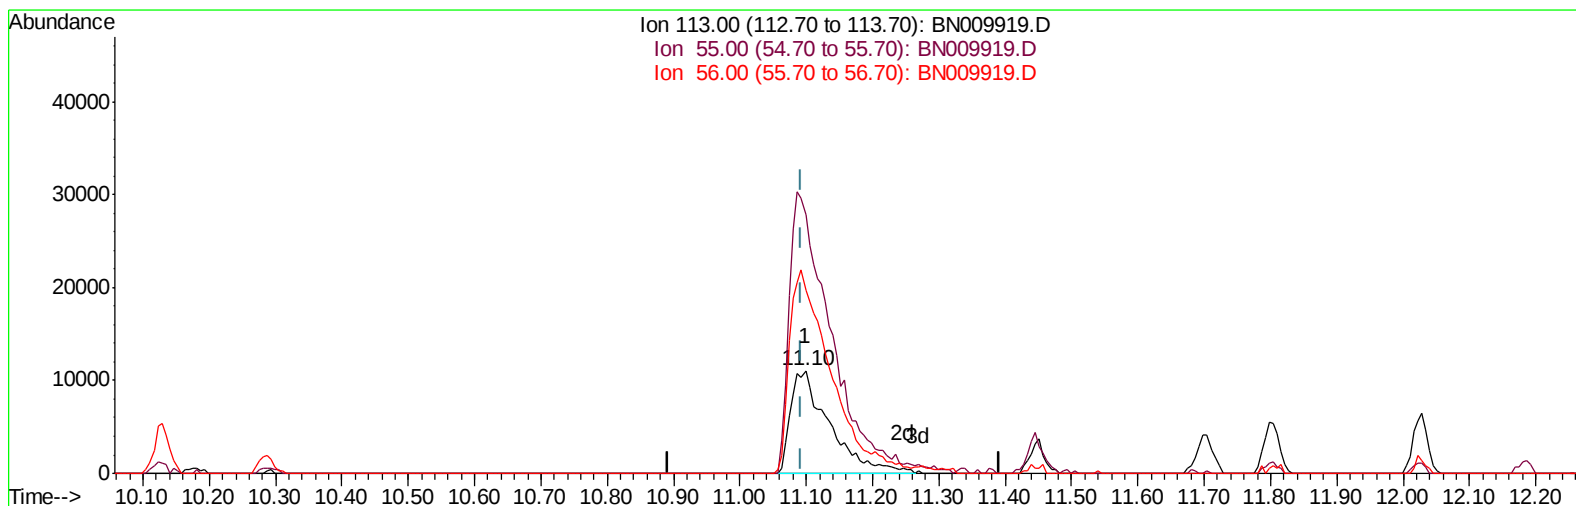

TIC: BN009919.D

(32) Caprolactam

11.099min (+0.006) 20.42ng/ul m

response 44480

Ion	Exp%	Act%
113.00	100	100
55.00	261.40	252.40
56.00	202.00	178.33
0.00	0.00	0.00