

Data File : BN009876.D
Acq On : 24 Feb 2020 22:52
Operator : CG/JU
Sample : L1582-18
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBDW3

Quant Time: Feb 25 02:42:43 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 25 02:39:29 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.39	152	92926	20.00	ng/ul	0.00
18) Naphthalene-d8	10.13	136	380947	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.03	164	240454	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.79	188	519105	20.00	ng/ul	0.00
78) Chrysene-d12	21.00	240	455556	20.00	ng/ul	0.00
86) Perylene-d12	23.10	264	543061	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.03	96	9987	4.42	ng/uL	0.00
5) Phenol-d5	6.59	99	51031	6.46	ng/ul	0.01
7) Bis-(2-Chloroethyl)ether-d	6.75	67	168914	30.97	ng/ul	0.00
9) 2-Chlorophenol-d4	6.93	132	150689	25.32	ng/ul	0.00
13) 4-Methylphenol-d8	8.10	113	99112	15.76	ng/ul	0.00
19) Nitrobenzene-d5	8.53	128	91416	32.80	ng/ul	0.01
22) 2-Nitrophenol-d4	9.24	143	96995	31.81	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.78	165	157968	26.95	ng/ul	0.00
29) 4-Chloroaniline-d4	10.33	131	10972	1.67	ng/ul	0.05
44) Dimethylphthalate-d6	13.46	166	624518	34.77	ng/ul	0.00
47) Acenaphthylene-d8	13.72	160	716366	33.87	ng/ul	0.00
52) 4-Nitrophenol-d4	14.29	143	10589	3.23	ng/ul	0.02
58) Fluorene-d10	15.03	176	561814	36.23	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.19	200	84534	26.21	ng/ul	0.00
71) Anthracene-d10	16.89	188	930959	39.12	ng/ul	0.00
79) Pyrene-d10	19.19	212	1052644	44.21	ng/ul	0.00
90) Benzo(a)pyrene-d12	22.97	264	1084306	39.98	ng/ul	0.00


Target Compounds					Qvalue	
45) Dimethylphthalate	13.50	163	34226	1.826	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN009876.D
Acq On : 24 Feb 2020 22:52
Operator : CG/JU
Sample : L1582-18
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBDW3

Quant Time: Feb 25 02:42:43 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 25 02:39:29 2020
Response via : Initial Calibration

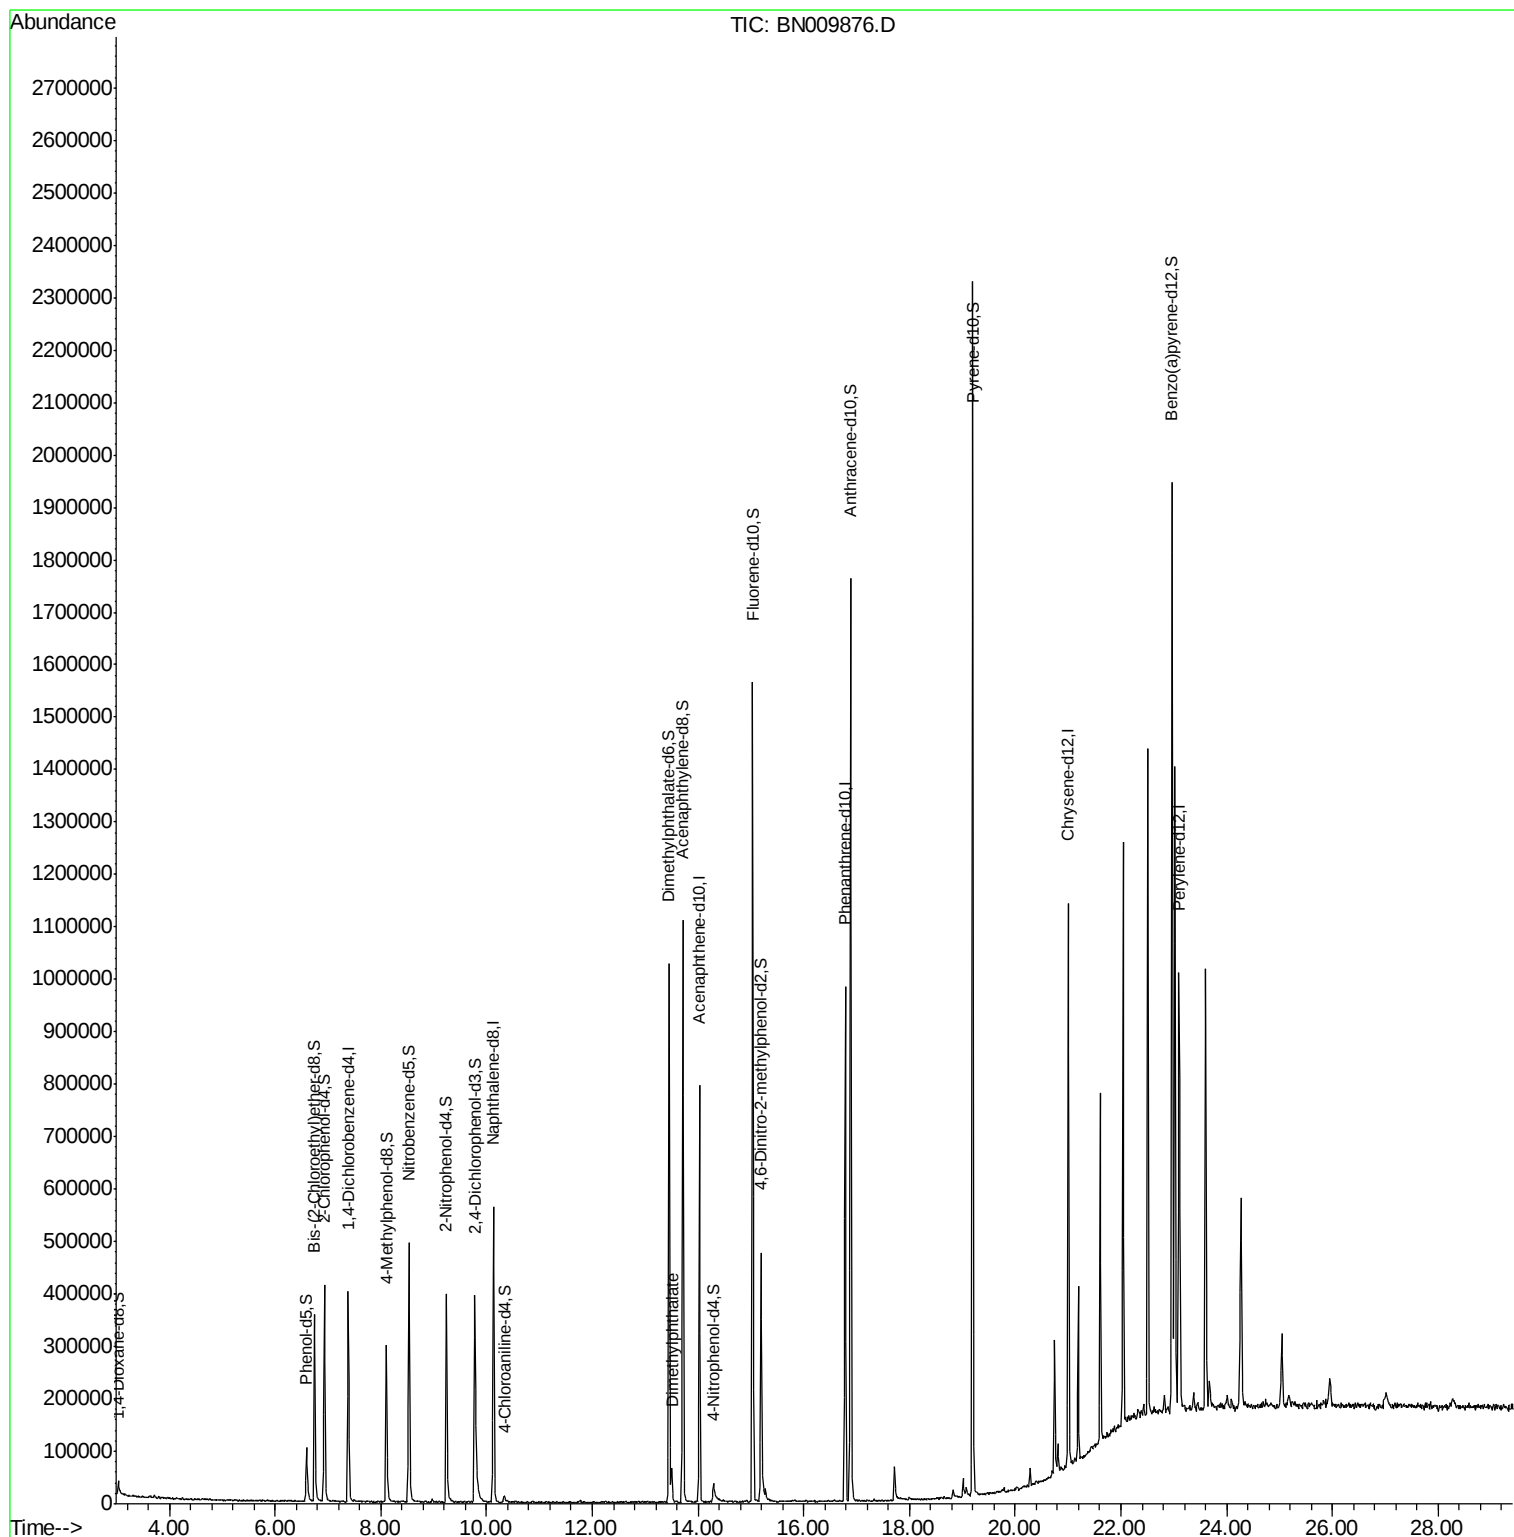

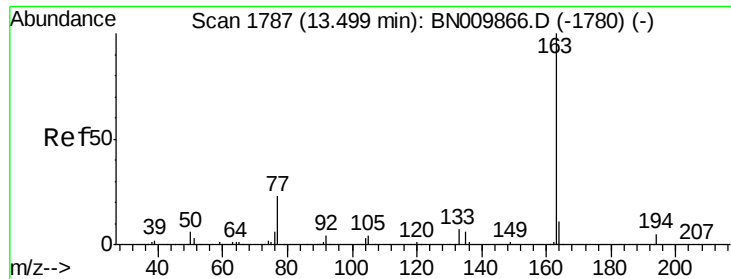

#45

Dimethylphthalate

Concen: 1.826 ng/ul

RT: 13.50 min Scan# 1788

Delta R.T. 0.01 min

Lab File: BN009876.D

Acq: 24 Feb 2020 22:52

Instrument :

BNA_N

ClientSampleId :

DBDW3


Tgt Ion:163 Resp: 34226

Ion Ratio Lower Upper

163 100

194 3.5 3.4 5.0

164 9.9 8.0 12.0

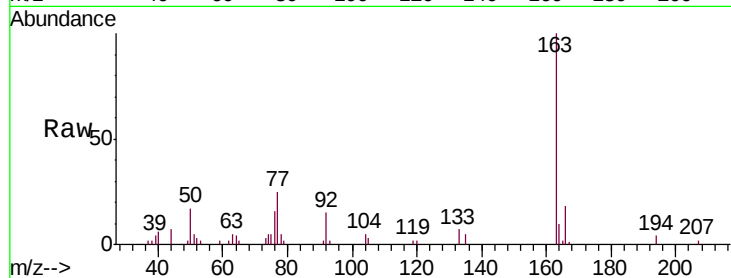

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

