

Data File : BN009886.D
Acq On : 25 Feb 2020 06:05
Operator : CG/JU
Sample : PB126940BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK40

Quant Time: Feb 25 07:24:52 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 25 07:22:29 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.39	152	127359	20.00	ng/ul	0.00
18) Naphthalene-d8	10.13	136	536386	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.03	164	334506	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.79	188	729737	20.00	ng/ul	0.00
78) Chrysene-d12	21.00	240	715754	20.00	ng/ul	0.00
86) Perylene-d12	23.10	264	719803	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.03	96	19733	6.37	ng/uL	0.00
5) Phenol-d5	6.59	99	338078	31.21	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.75	67	246091	32.92	ng/ul	0.00
9) 2-Chlorophenol-d4	6.93	132	270732	33.20	ng/ul	0.00
13) 4-Methylphenol-d8	8.10	113	274942	31.91	ng/ul	0.00
19) Nitrobenzene-d5	8.53	128	132429	33.75	ng/ul	0.00
22) 2-Nitrophenol-d4	9.24	143	148805	34.66	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.78	165	253819	30.75	ng/ul	0.00
29) 4-Chloroaniline-d4	10.29	131	362005	39.04	ng/ul	0.00
44) Dimethylphthalate-d6	13.45	166	834034	33.38	ng/ul	0.00
47) Acenaphthylene-d8	13.71	160	982501	33.39	ng/ul	0.00
52) 4-Nitrophenol-d4	14.27	143	121014	26.52	ng/ul	0.00
58) Fluorene-d10	15.03	176	718507	33.31	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.19	200	111677	24.64	ng/ul	0.00
71) Anthracene-d10	16.88	188	1095218	32.74	ng/ul	0.00
79) Pyrene-d10	19.19	212	1210127	32.35	ng/ul	0.00
90) Benzo(a)pyrene-d12	22.97	264	1214006	33.77	ng/ul	0.00


Target Compounds				Qvalue		
15) N-Nitroso-di-n-propylamine	8.10	70	8165	1.113	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN009886.D
Acq On : 25 Feb 2020 06:05
Operator : CG/JU
Sample : PB126940BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK40

Quant Time: Feb 25 07:24:52 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 25 07:22:29 2020
Response via : Initial Calibration

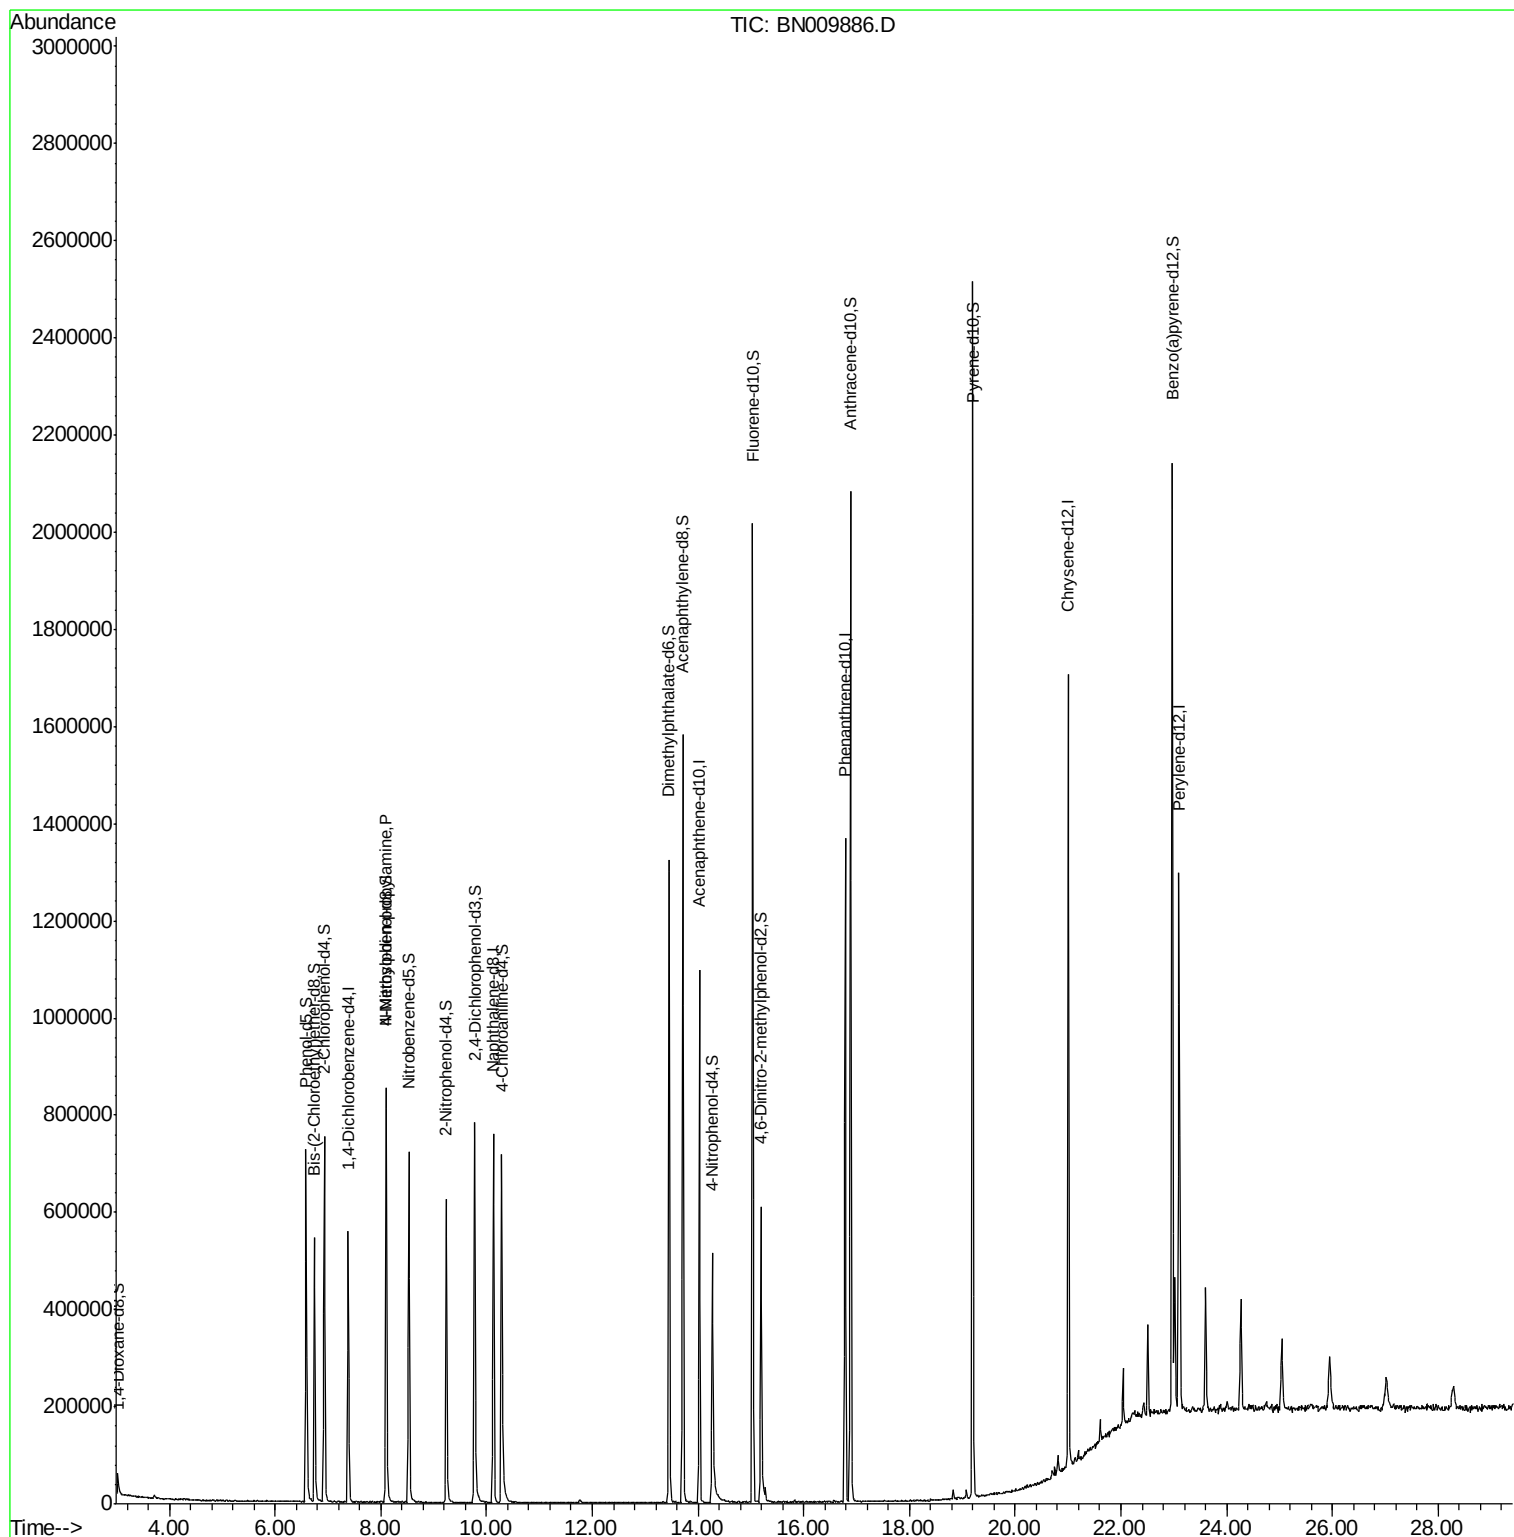

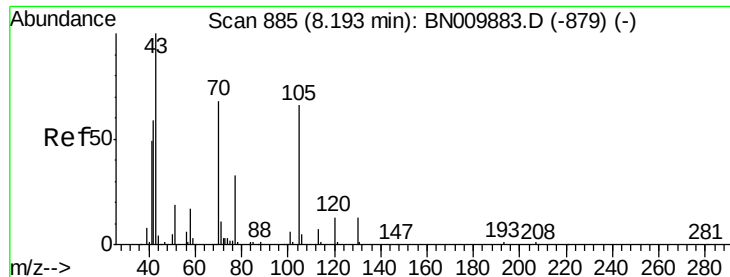

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.113 ng/ul
 RT: 8.10 min Scan# 870
 Delta R.T. -0.09 min
 Lab File: BN009886.D
 Acq: 25 Feb 2020 06:05

Instrument :
 BNA_N
 ClientSampleId :
 SBLK40

Tgt Ion: 70 Resp: 8165
 Ion Ratio Lower Upper
 70 100
 42 536.6 72.6 108.8#
 101 0.0 7.7 11.5#
 130 0.0 14.7 22.1#

