

Data File : BN009900.D
Acq On : 25 Feb 2020 14:29
Operator : CG/JU
Sample : PB126804BL
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK04

Quant Time: Feb 26 07:09:46 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 26 07:04:59 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.39	152	98559	20.00	ng/ul	0.00
18) Naphthalene-d8	10.13	136	417582	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.03	164	256767	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.78	188	555926	20.00	ng/ul	0.00
78) Chrysene-d12	21.00	240	555474	20.00	ng/ul	0.00
86) Perylene-d12	23.10	264	577641	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.03	96	16709	6.97	ng/uL	0.00
5) Phenol-d5	6.59	99	263706	31.45	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.75	67	191451	33.09	ng/ul	0.00
9) 2-Chlorophenol-d4	6.93	132	211356	33.49	ng/ul	0.00
13) 4-Methylphenol-d8	8.10	113	208218	31.22	ng/ul	0.00
19) Nitrobenzene-d5	8.53	128	100665	32.95	ng/ul	0.00
22) 2-Nitrophenol-d4	9.24	143	110733	33.13	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.78	165	199325	31.02	ng/ul	0.00
29) 4-Chloroaniline-d4	10.29	131	270135	37.42	ng/ul	0.00
44) Dimethylphthalate-d6	13.46	166	623766	32.52	ng/ul	0.00
47) Acenaphthylene-d8	13.71	160	739601	32.74	ng/ul	0.00
52) 4-Nitrophenol-d4	14.27	143	78816	22.50	ng/ul	0.00
58) Fluorene-d10	15.03	176	544892	32.91	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.19	200	75239	21.79	ng/ul	0.00
71) Anthracene-d10	16.89	188	825422	32.39	ng/ul	0.00
79) Pyrene-d10	19.19	212	915624	31.54	ng/ul	0.00
90) Benzo(a)pyrene-d12	22.97	264	966731	33.51	ng/ul	0.00


Target Compounds					Qvalue	
15) N-Nitroso-di-n-propylamine	8.10	70	6154	1.084	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN009900.D
Acq On : 25 Feb 2020 14:29
Operator : CG/JU
Sample : PB126804BL
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK04

Quant Time: Feb 26 07:09:46 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 26 07:04:59 2020
Response via : Initial Calibration

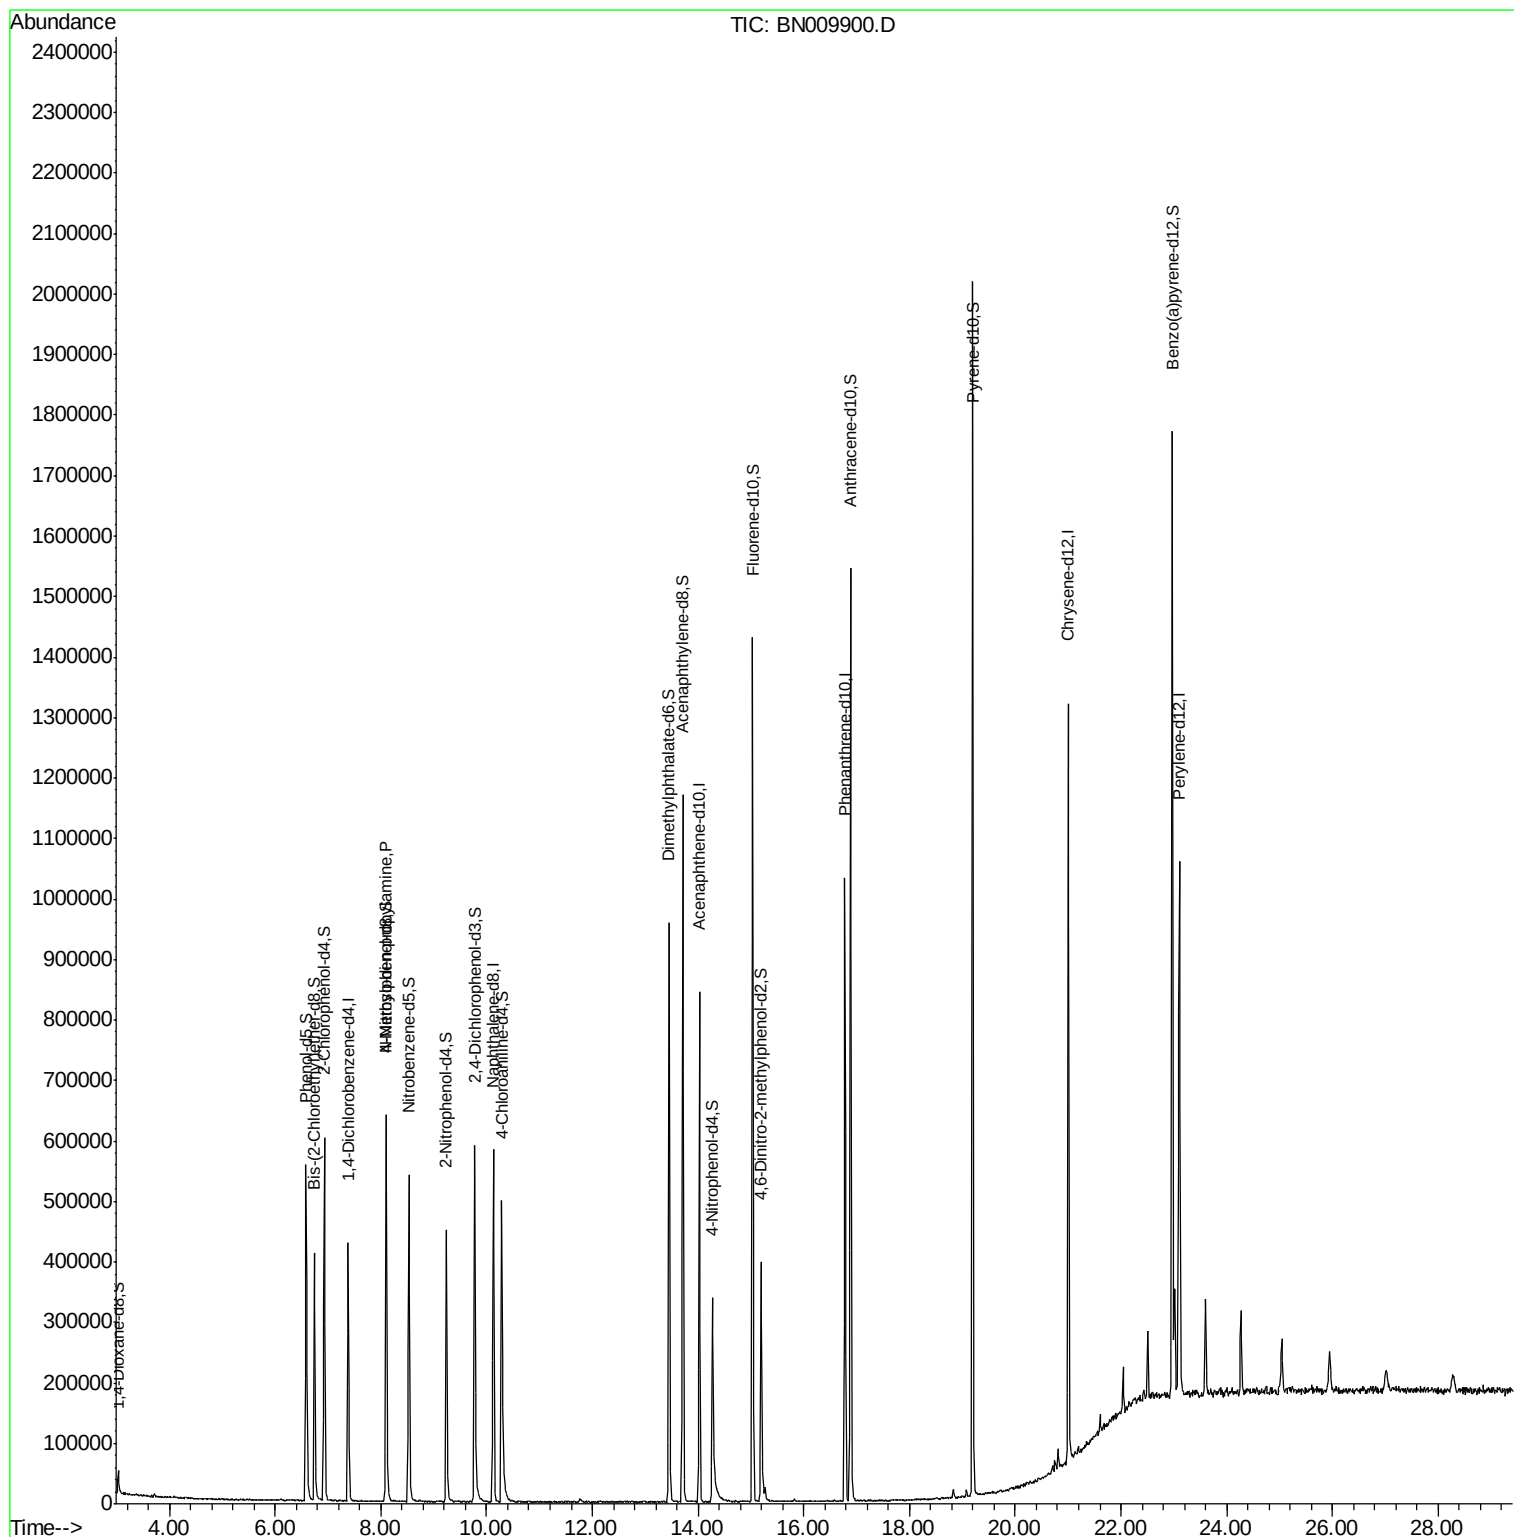

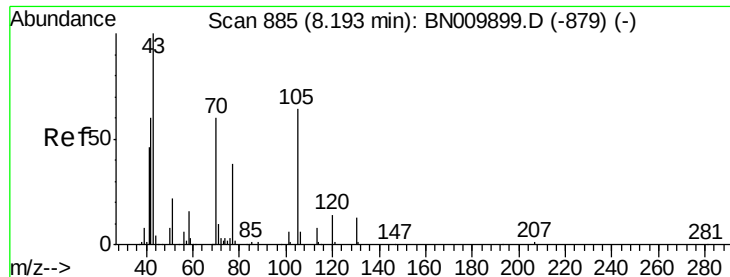

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.084 ng/ul
 RT: 8.10 min Scan# 869
 Delta R.T. -0.09 min
 Lab File: BN009900.D
 Acq: 25 Feb 2020 14:29

Instrument :
 BNA_N
 ClientSampleId :
 SBLK04

Tgt Ion: 70 Resp: 6154
 Ion Ratio Lower Upper
 70 100
 42 562.2 72.6 108.8#
 101 0.0 7.7 11.5#
 130 0.0 14.7 22.1#

