

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN022420\
 Data File : BN009892.D
 Acq On : 25 Feb 2020 09:40
 Operator : CG/JU
 Sample : L1486-22DL2 150X
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBCX4DL2

Quant Time: Feb 25 13:55:47 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 25 07:22:29 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.39	152	88430	20.00	ng/ul	0.00
18) Naphthalene-d8	10.13	136	379693	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.03	164	244002	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.79	188	518474	20.00	ng/ul	0.00
78) Chrysene-d12	21.00	240	495648	20.00	ng/ul	0.00
86) Perylene-d12	23.10	264	496534	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	0.00	96	0	0.00	ng/uL	
5) Phenol-d5	0.00	99	0	0.00	ng/ul	
7) Bis-(2-Chloroethyl)ether-d	0.00	67	0d	0.00	ng/ul	
9) 2-Chlorophenol-d4	0.00	132	0	0.00	ng/ul	
13) 4-Methylphenol-d8	0.00	113	0	0.00	ng/ul	
19) Nitrobenzene-d5	0.00	128	0	0.00	ng/ul	
22) 2-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
26) 2,4-Dichlorophenol-d3	0.00	165	0	0.00	ng/ul	
29) 4-Chloroaniline-d4	0.00	131	0	0.00	ng/ul	
44) Dimethylphthalate-d6	13.49	166	3140	0.17	ng/ul	0.04
47) Acenaphthylene-d8	13.72	160	4523	0.21	ng/ul	0.01
52) 4-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
58) Fluorene-d10	15.05	176	3499	0.22	ng/ul	0.01
63) 4,6-Dinitro-2-methylphenol	0.00	200	0	0.00	ng/ul	
71) Anthracene-d10	16.90	188	6772	0.28	ng/ul	0.02
79) Pyrene-d10	19.20	212	7367	0.28	ng/ul	0.01
90) Benzo(a)pyrene-d12	22.97	264	5814	0.23	ng/ul	0.00

Target Compounds


					Ovalue	
28) Naphthalene	10.18	128	784127	38.297	ng/ul	99
50) Acenaphthene	14.09	153	28899	1.814	ng/ul	89
54) Dibenzofuran	14.45	168	42952	1.921	ng/ul	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN022420\
Data File : BN009892.D
Acq On : 25 Feb 2020 09:40
Operator : CG/JU
Sample : L1486-22DL2 150X
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBCX4DL2

Quant Time: Feb 25 13:55:47 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 25 07:22:29 2020
Response via : Initial Calibration

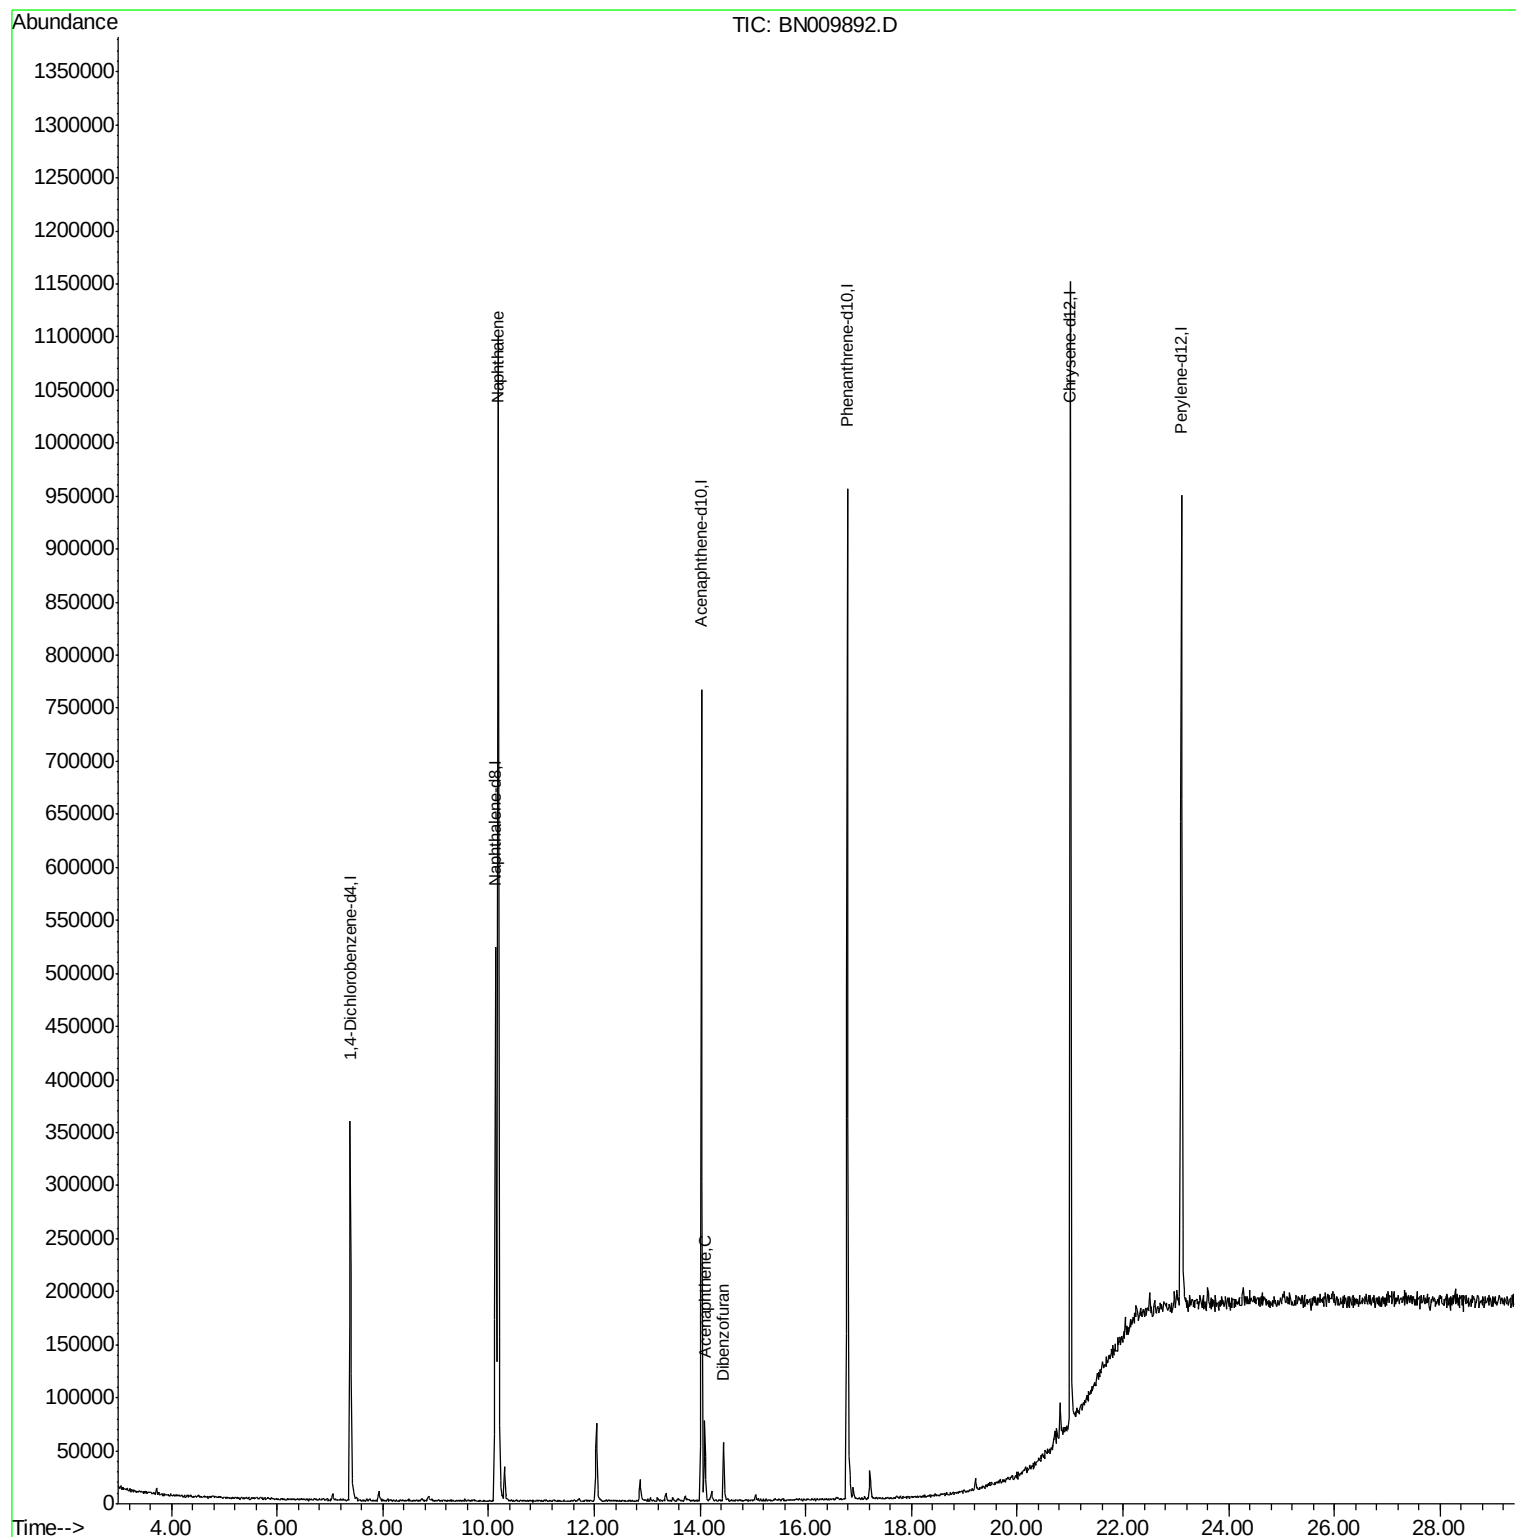

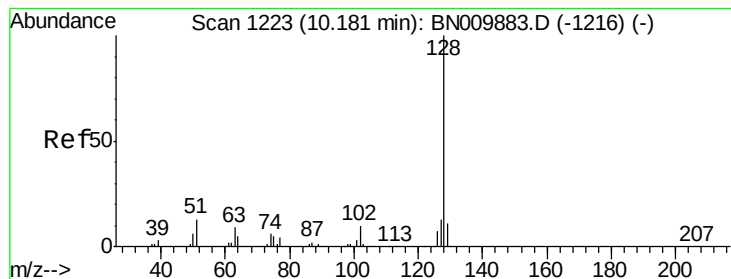

#28

Naphthalene

Concen: 38.297 ng/ul

RT: 10.18 min Scan# 1223

Delta R.T. -0.00 min

Lab File: BN009892.D

Acq: 25 Feb 2020 09:40

Instrument :

BNA_N

ClientSampleId :

DBCX4DL2


Tot Ion:128 Resp: 784127

Ion Ratio Lower Upper

128 100

129 11.3 8.6 13.0




127 13.3 10.3 15.5

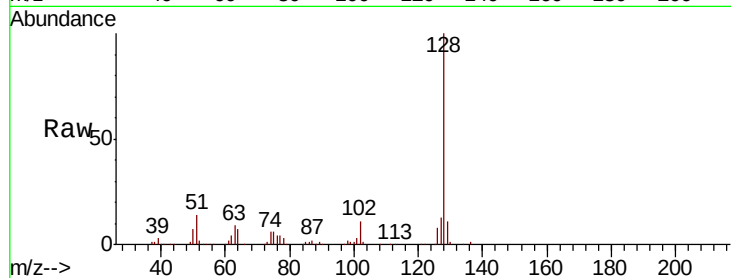

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

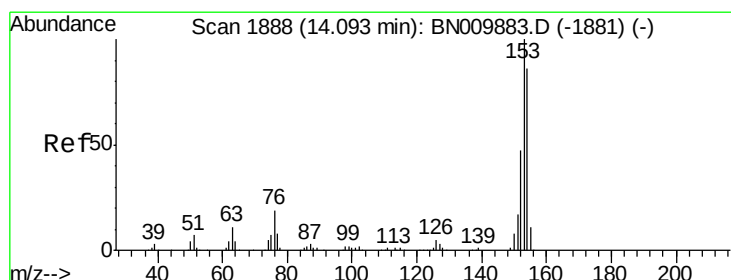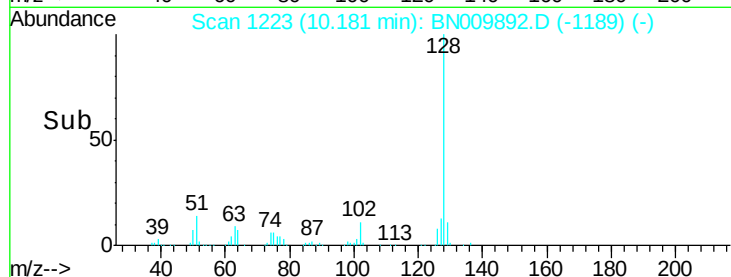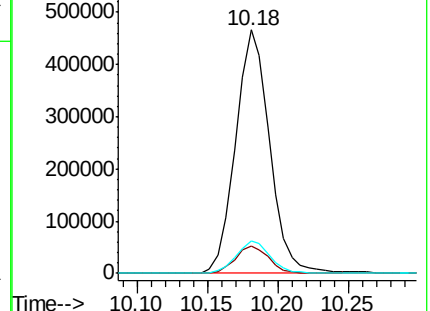

#50

Acenaphthene

Concen: 1.814 ng/ul

RT: 14.09 min Scan# 1888

Delta R.T. -0.00 min

Lab File: BN009892.D

Acq: 25 Feb 2020 09:40


Tgt Ion:153 Resp: 28899

Ion Ratio Lower Upper

153 100

152 48.3 36.6 54.8



154 101.3 70.6 106.0

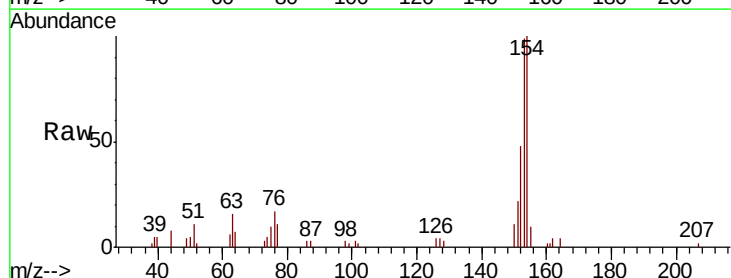


Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

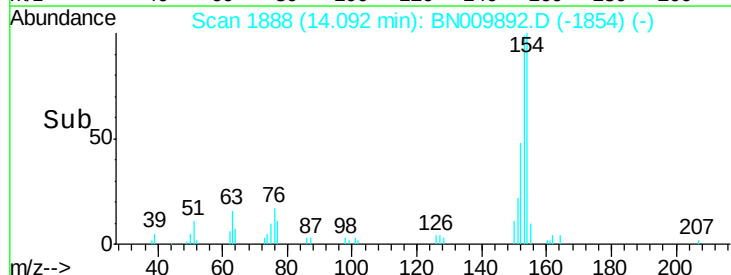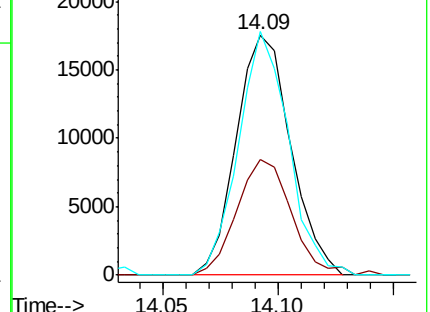

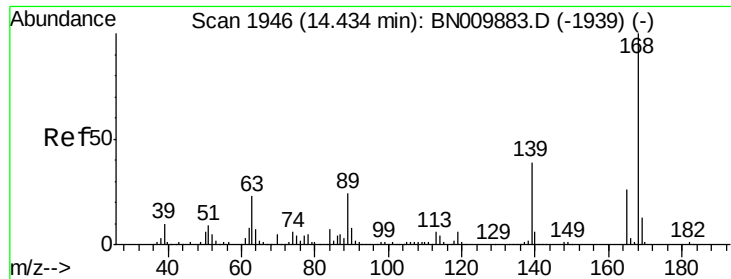

#54

Dibenzofuran

Concen: 1.921 ng/ul

RT: 14.45 min Scan# 1948

Delta R.T. 0.01 min

Lab File: BN009892.D

Acq: 25 Feb 2020 09:40

Instrument :

BNA_N

ClientSampleId :

DBCX4DL2

Tot Ion:168 Resp: 42952

Ion Ratio Lower Upper

168 100

139 38.6 32.7 49.1

