

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN022420\
 Data File : BN009917.D
 Acq On : 26 Feb 2020 01:20
 Operator : CG/JU
 Sample : L1568-12
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBDB3

Quant Time: Feb 26 08:13:55 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Feb 26 07:56:07 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.38	152	100428	20.00	ng/ul	0.00
18) Naphthalene-d8	10.13	136	417186	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.02	164	255555	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.78	188	548222	20.00	ng/ul	0.00
78) Chrysene-d12	21.00	240	547233	20.00	ng/ul	0.00
86) Perylene-d12	23.09	264	545118	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.03	96	9710	3.98	ng/uL	0.00
5) Phenol-d5	6.59	99	189280	22.16	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.74	67	140105	23.77	ng/ul	0.00
9) 2-Chlorophenol-d4	6.93	132	158880	24.71	ng/ul	0.00
13) 4-Methylphenol-d8	8.10	113	147838	21.76	ng/ul	0.00
19) Nitrobenzene-d5	8.53	128	77254	25.31	ng/ul	0.00
22) 2-Nitrophenol-d4	9.24	143	83144	24.90	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.78	165	157343	24.51	ng/ul	0.00
29) 4-Chloroaniline-d4	10.29	131	177457	24.61	ng/ul	0.00
44) Dimethylphthalate-d6	13.45	166	531783	27.86	ng/ul	0.00
47) Acenaphthylene-d8	13.71	160	614516	27.33	ng/ul	0.00
52) 4-Nitrophenol-d4	14.28	143	74859	21.47	ng/ul	0.00
58) Fluorene-d10	15.03	176	447441	27.15	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.19	200	67456	19.81	ng/ul	0.00
71) Anthracene-d10	16.88	188	727483	28.95	ng/ul	0.00
79) Pyrene-d10	19.19	212	819185	28.64	ng/ul	0.00
90) Benzo(a)pyrene-d12	22.97	264	840069	30.86	ng/ul	0.00


Target Compounds					Ovalue
45) Dimethylphthalate	13.50	163	73630	3.697	ng/ul 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN022420\
Data File : BN009917.D
Acq On : 26 Feb 2020 01:20
Operator : CG/JU
Sample : L1568-12
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBDB3

Quant Time: Feb 26 08:13:55 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 26 07:56:07 2020
Response via : Initial Calibration

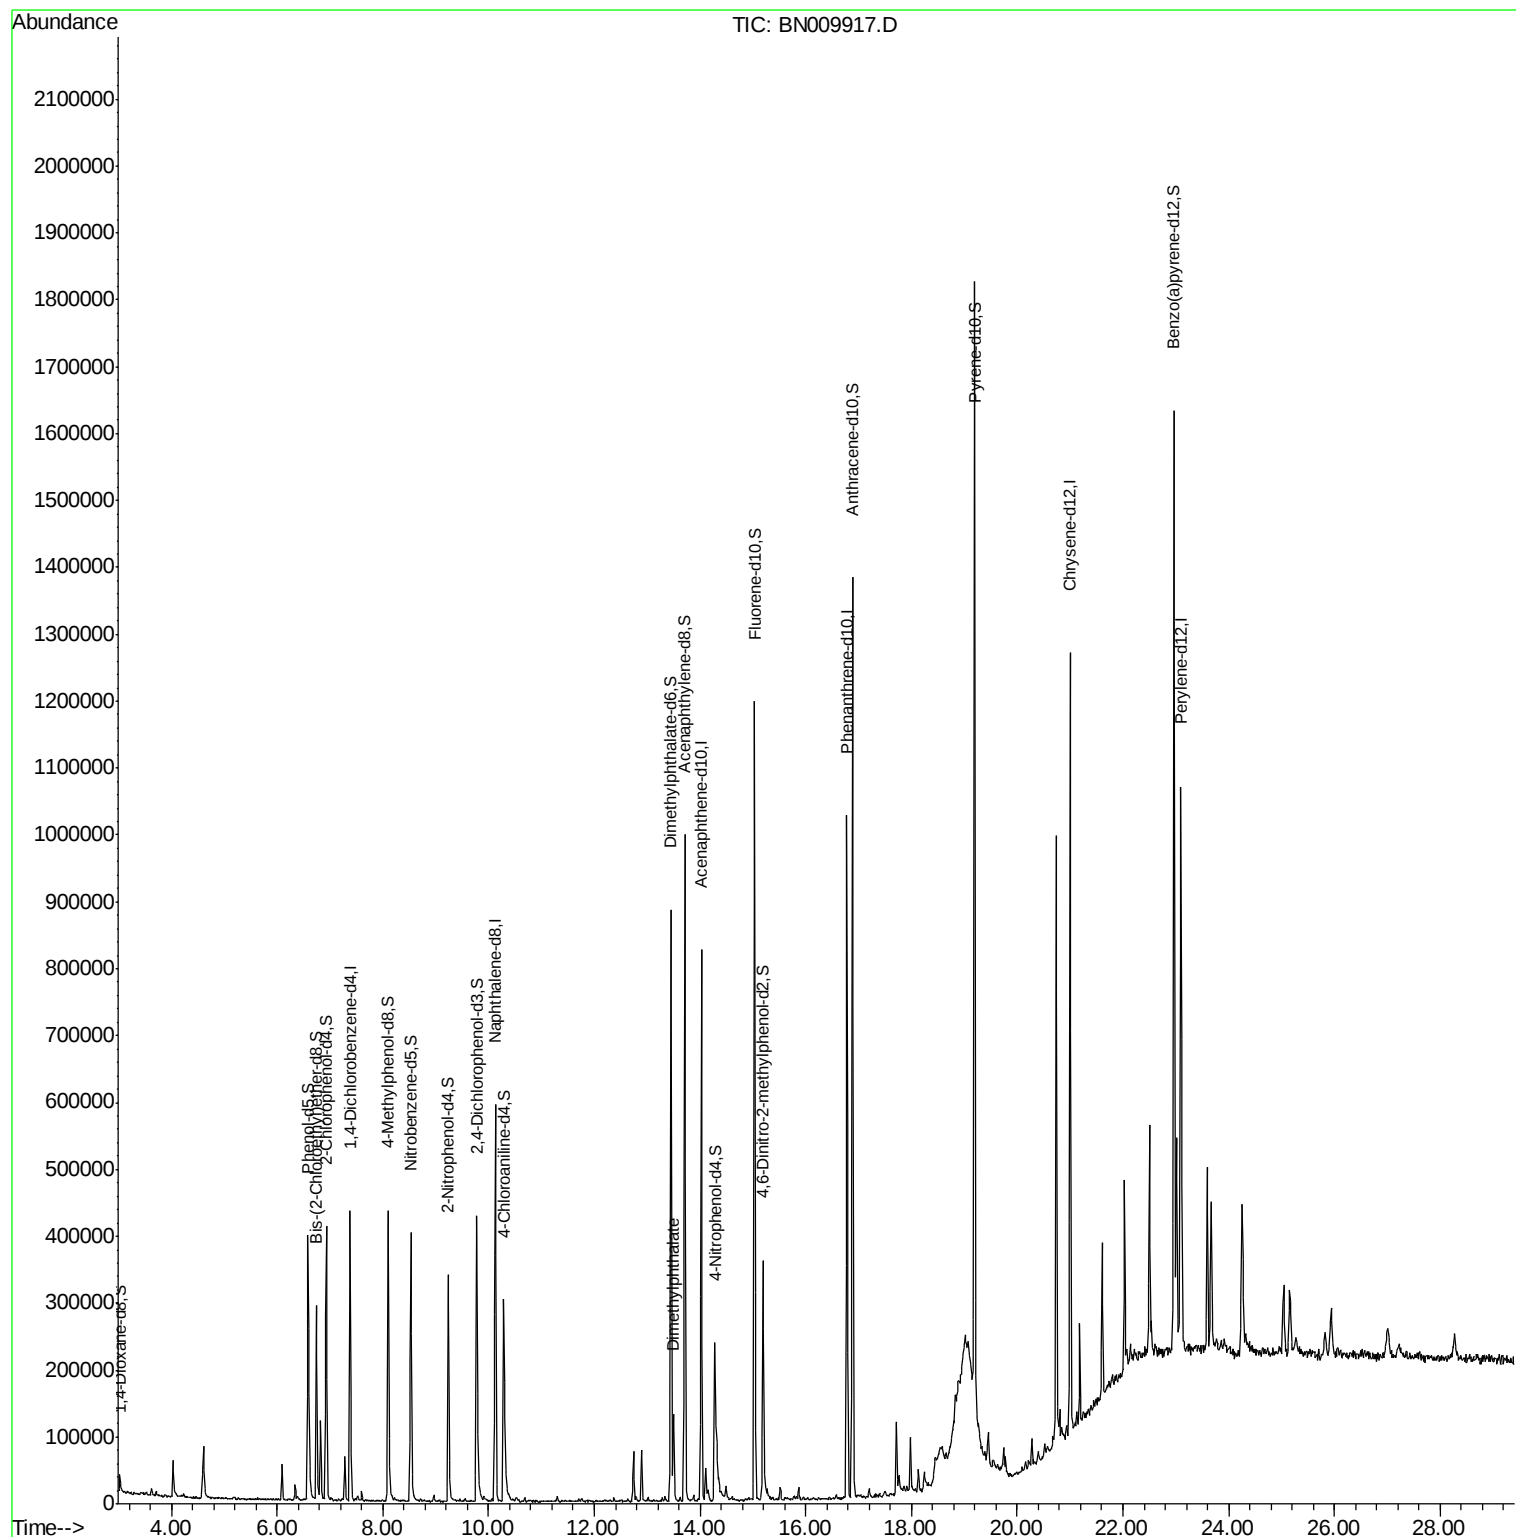

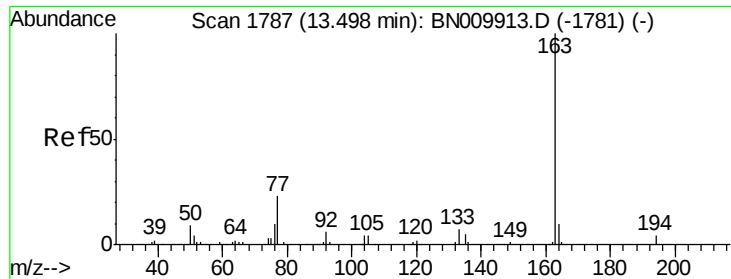

#45

Dimethylphthalate

Concen: 3.697 ng/ul

RT: 13.50 min Scan# 1787

Delta R.T. 0.00 min

Lab File: BN009917.D

Acq: 26 Feb 2020 01:20

Instrument :

BNA_N

ClientSampleId :

DBDB3


Tot Ion:163 Resp: 73630

Ion Ratio Lower Upper

163 100

194 4.1 3.4 5.0

164 10.8 8.0 12.0

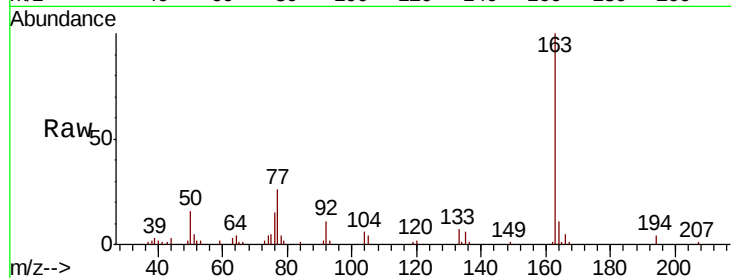

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

