

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN022420\
 Data File : BN009892.D
 Acq On : 25 Feb 2020 09:40
 Operator : CG/JU
 Sample : L1486-22DL2 150X
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBCX4DL2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	45	47	50	rVB3	2550	2739	0.15%	0.029%
2	3.499	85	87	90	rBV3	1935	2435	0.13%	0.026%
3	3.716	121	124	127	rVB4	5996	8170	0.43%	0.086%
4	3.875	148	151	153	rBV4	1809	1949	0.10%	0.021%
5	4.416	239	243	245	rBV3	2144	2948	0.16%	0.031%
6	4.699	288	291	292	rBV3	1706	2200	0.12%	0.023%
7	5.040	346	349	351	rVB3	1658	2000	0.11%	0.021%
8	5.522	426	431	432	rBV4	2337	2824	0.15%	0.030%
9	5.934	500	501	505	rVB2	2021	2066	0.11%	0.022%
10	6.316	564	566	569	rBV2	1940	2199	0.12%	0.023%
11	7.052	686	691	696	rVV3	6402	10303	0.55%	0.109%
12	7.322	734	737	740	rBV3	2001	3147	0.17%	0.033%
13	7.387	742	748	764	rVV	357974	619389	32.88%	6.530%
14	7.499	764	767	772	rVB5	3206	5979	0.32%	0.063%
15	7.752	807	810	814	rVB	2599	3574	0.19%	0.038%
16	7.922	834	839	847	rBV6	10315	19783	1.05%	0.209%
17	8.740	973	978	980	rBV5	3000	4288	0.23%	0.045%
18	8.869	993	1000	1005	rVV5	5295	11592	0.62%	0.122%
19	9.063	1030	1033	1038	rVB4	1861	2806	0.15%	0.030%
20	9.151	1044	1048	1051	rBV3	1534	1964	0.10%	0.021%
21	9.546	1113	1115	1119	rVV3	1667	2100	0.11%	0.022%
22	9.834	1157	1164	1167	rVV2	1064	2093	0.11%	0.022%
23	10.134	1208	1215	1218	rVV	522352	843497	44.78%	8.893%
24	10.181	1218	1223	1235	rVV	1097849	1883770	100.00%	19.861%
25	10.304	1238	1244	1250	rVV	32179	58893	3.13%	0.621%
26	10.351	1250	1252	1255	rVV2	2392	3013	0.16%	0.032%
27	11.704	1474	1482	1491	rVB6	2875	7112	0.38%	0.075%
28	11.934	1517	1521	1524	rBV3	1438	2502	0.13%	0.026%
29	12.040	1530	1539	1554	rBV2	74127	154024	8.18%	1.624%
30	12.863	1673	1679	1687	rBV2	20797	39211	2.08%	0.413%
31	13.057	1708	1712	1719	rBV2	3112	4496	0.24%	0.047%
32	13.192	1732	1735	1737	rBV3	3333	3847	0.20%	0.041%
33	13.357	1758	1763	1766	rBV5	6824	11964	0.64%	0.126%
34	13.487	1779	1785	1788	rBV3	3709	6123	0.33%	0.065%

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN022420\
 Data File : BN009892.D
 Acq On : 25 Feb 2020 09:40
 Operator : CG/JU
 Sample : L1486-22DL2 150X
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DBCX4DL2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
 Title : SVOA CALIBRATION

35	13.716	1820	1824	1829	rVV2	4900	6942	0.37%	0.073%
36	14.028	1870	1877	1884	rBV	765255	1139791	60.51%	12.017%
37	14.092	1884	1888	1900	rVB2	76777	121138	6.43%	1.277%
38	14.169	1900	1901	1903	rBV2	2308	1950	0.10%	0.021%
39	14.216	1903	1909	1918	rVV3	9222	19834	1.05%	0.209%
40	14.445	1942	1948	1958	rBV	55347	97680	5.19%	1.030%
41	15.045	2047	2050	2056	rVB2	5840	9726	0.52%	0.103%
42	15.104	2056	2060	2063	rVB4	1762	2904	0.15%	0.031%
43	15.298	2089	2093	2095	rBV2	1499	2363	0.13%	0.025%
44	15.404	2108	2111	2113	rBV4	2040	2479	0.13%	0.026%
45	15.563	2135	2138	2141	rBV3	1697	1898	0.10%	0.020%
46	16.169	2237	2241	2243	rVB2	1485	1962	0.10%	0.021%
47	16.575	2307	2310	2313	rBV2	2081	3465	0.18%	0.037%
48	16.786	2340	2346	2352	rBV	951540	1338529	71.06%	14.112%
49	16.898	2361	2365	2370	rVB2	9883	13947	0.74%	0.147%
50	17.216	2414	2419	2426	rBV2	27575	47171	2.50%	0.497%
51	17.539	2471	2474	2478	rVB4	1735	2573	0.14%	0.027%
52	17.710	2498	2503	2506	rBV3	2292	3921	0.21%	0.041%
53	17.792	2514	2517	2519	rVB2	2264	2433	0.13%	0.026%
54	17.945	2540	2543	2546	rVV3	2050	2674	0.14%	0.028%
55	18.098	2568	2569	2573	rBV2	1665	2150	0.11%	0.023%
56	18.257	2595	2596	2599	rVB2	2431	1885	0.10%	0.020%
57	18.310	2602	2605	2608	rBV3	1252	2109	0.11%	0.022%
58	18.769	2682	2683	2686	rBV3	1832	2125	0.11%	0.022%
59	18.980	2718	2719	2722	rBV3	2428	2942	0.16%	0.031%
60	19.204	2754	2757	2763	rBV4	10152	14762	0.78%	0.156%
61	19.404	2789	2791	2794	rBV3	3772	3717	0.20%	0.039%
62	19.480	2802	2804	2806	rVB2	3465	1947	0.10%	0.021%
63	19.998	2890	2892	2894	rVB3	6909	6398	0.34%	0.067%
64	20.021	2894	2896	2898	rBV3	7373	7376	0.39%	0.078%
65	20.186	2922	2924	2925	rBV	5400	4081	0.22%	0.043%
66	20.810	3027	3030	3034	rBV2	33798	48360	2.57%	0.510%
67	21.004	3058	3063	3074	rBV	1080046	1456169	77.30%	15.353%
68	23.104	3414	3420	3431	rVB	758209	1372409	72.85%	14.470%


Sum of corrected areas: 9484810

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN022420\
Data File : BN009892.D
Acq On : 25 Feb 2020 09:40
Operator : CG/JU
Sample : L1486-22DL2 150X
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBCX4DL2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

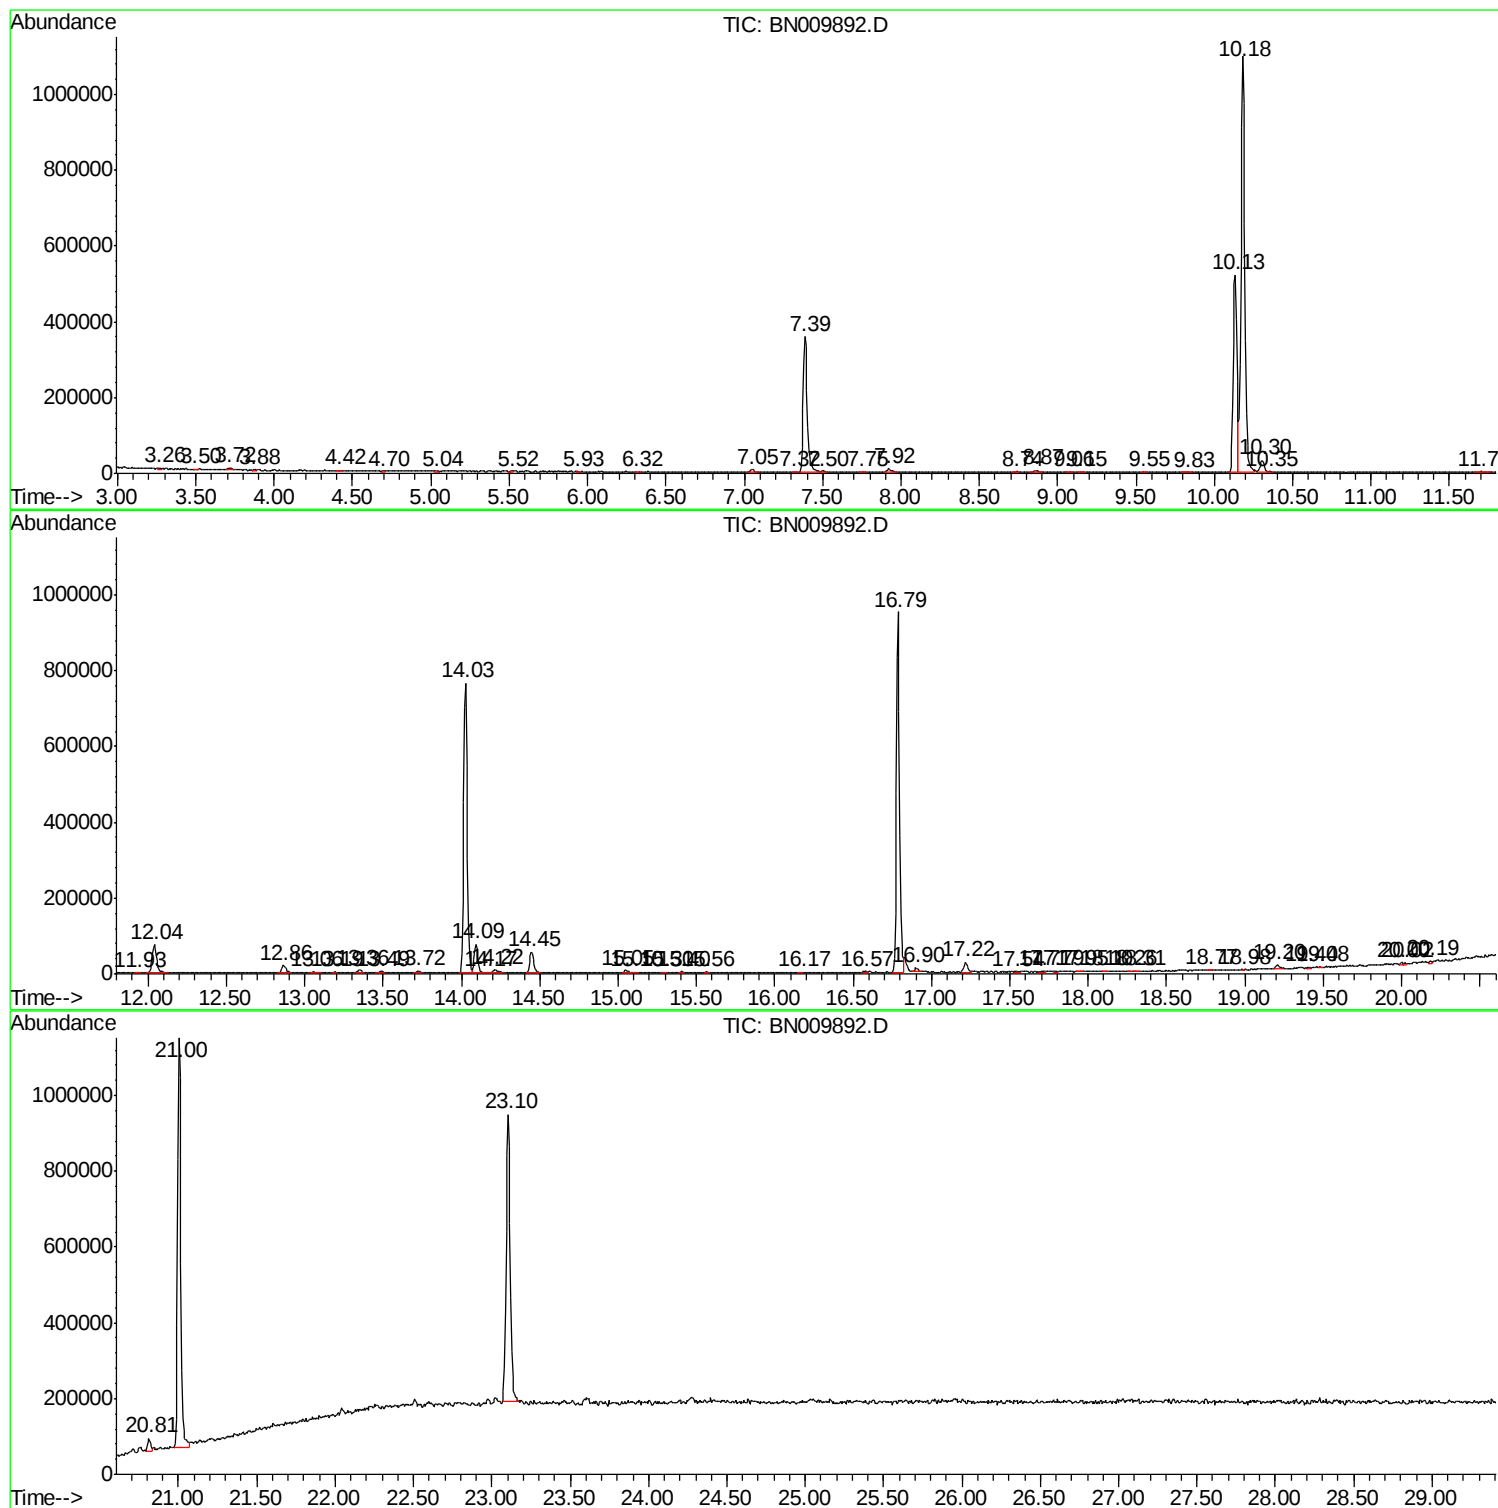

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN022420\
Data File : BN009892.D
Acq On : 25 Feb 2020 09:40
Operator : CG/JU
Sample : L1486-22DL2 150X
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBCX4DL2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN022420\
Data File : BN009892.D
Acq On : 25 Feb 2020 09:40
Operator : CG/JU
Sample : L1486-22DL2 150X
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DBCX4DL2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN021220MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc