
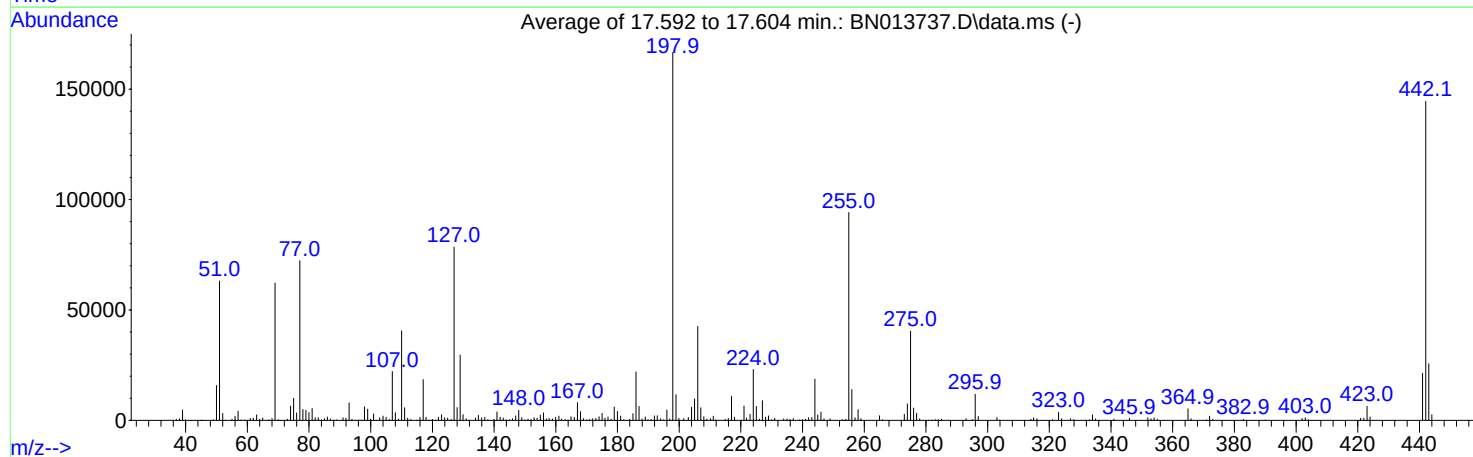


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022421\
 Data File : BN013737.D
 Acq On : 24 Feb 2021 16:42
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN022421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Feb 25 11:31:11 2021

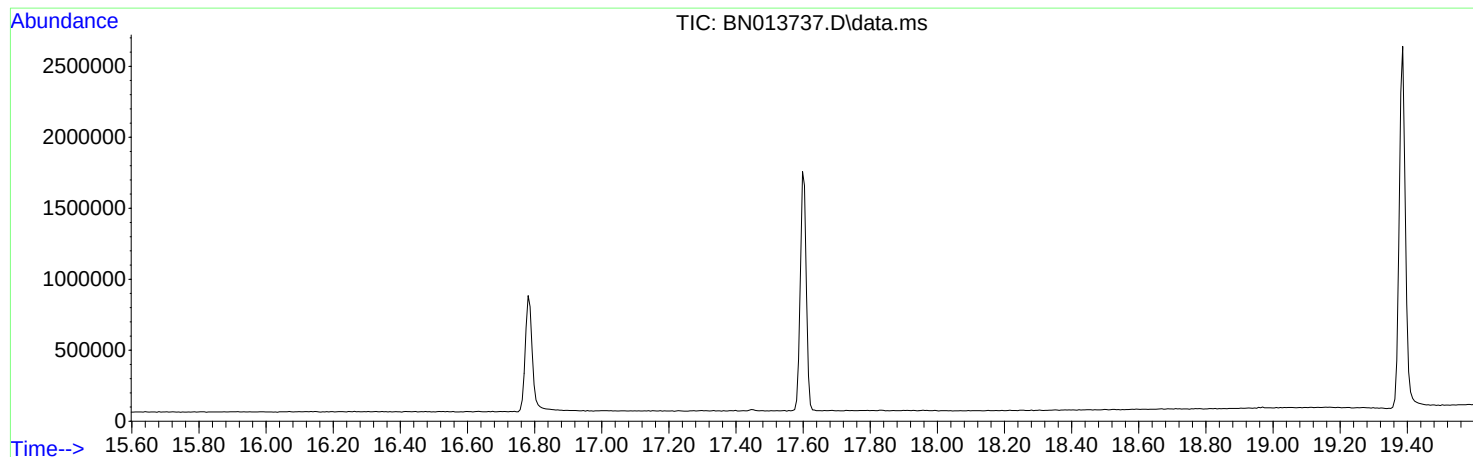

AutoFind: Scans 2466, 2467, 2468; Background Corrected with Scan 2460

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.9	63143	PASS
68	69	0.00	2	1.4	857	PASS
69	198	0.00	100	37.3	62179	PASS
70	69	0.00	2	0.5	318	PASS
127	198	10	80	47.1	78517	PASS
197	198	0.00	2	0.4	626	PASS
198	198	100	100	100.0	166613	PASS
199	198	5	9	7.0	11612	PASS
275	198	10	60	24.3	40475	PASS
365	198	1	100	3.1	5185	PASS
441	198	0.01	100	12.8	21306	PASS
442	442	50	100	100.0	144520	PASS
443	442	15	24	17.8	25674	PASS

DDT Breakdown




Instrument :
BNA_N
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
2/24/2021	BNA_N	<u>BN013737.D</u>
Compound Name	Response	Retention Time
DDT	474529	20.628
DDD	2124	20.239
DDE	5219	17.598
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7343	481872	1.52

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022421\
 Data File : BN013737.D
 Acq On : 24 Feb 2021 16:42
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Feb 26 06:45:28 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 26 06:45:22 2021
 Response via : Initial Calibration

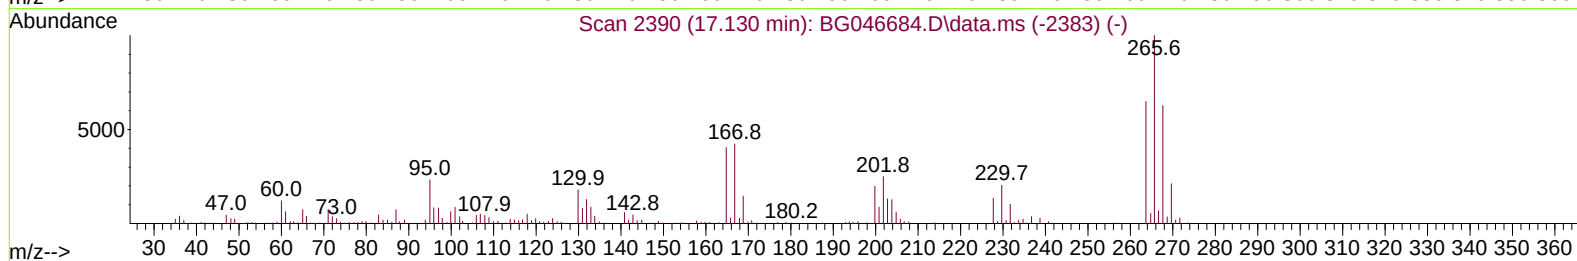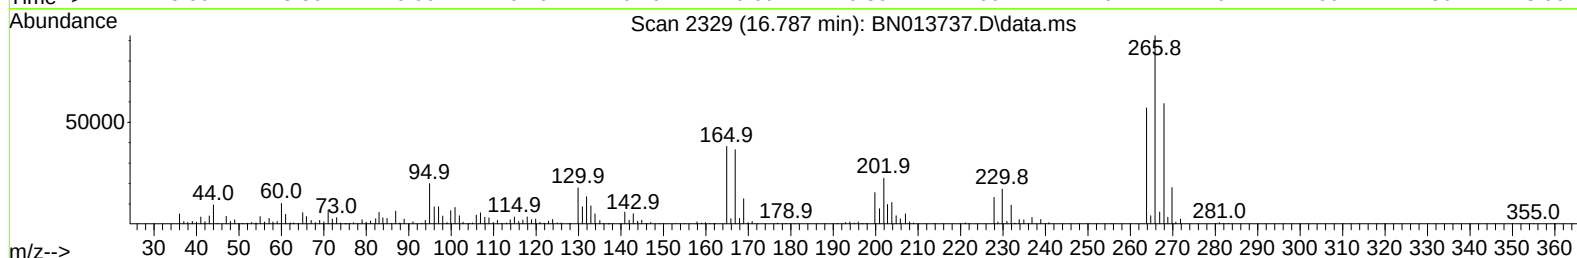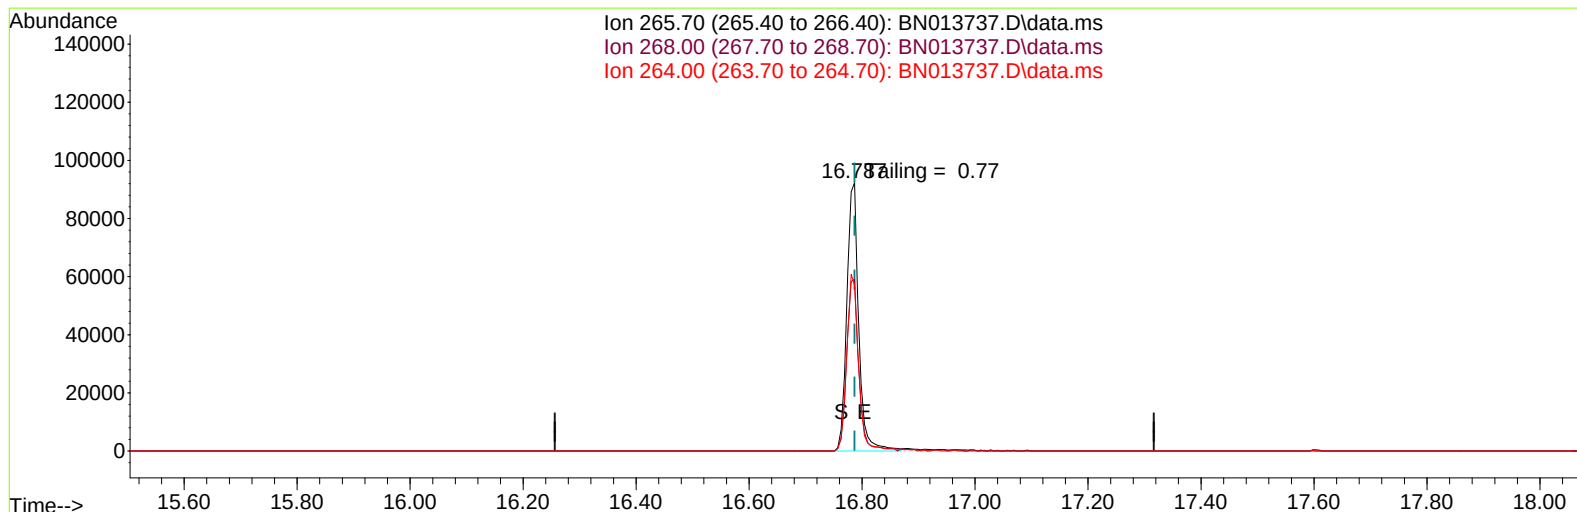

TIC: BN013737.D\data.ms

(70) Pentachlorophenol (C)

16.787min (0.000) 19578.47 ng




response 134902

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.02
264.00	61.60	61.75
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022421\
Data File : BN013737.D
Acq On : 24 Feb 2021 16:42
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Feb 26 06:45:28 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 26 06:45:22 2021
Response via : Initial Calibration

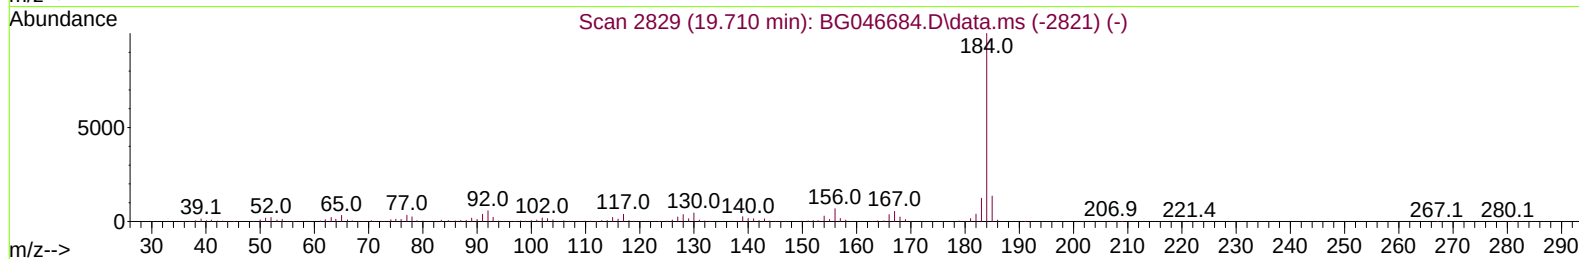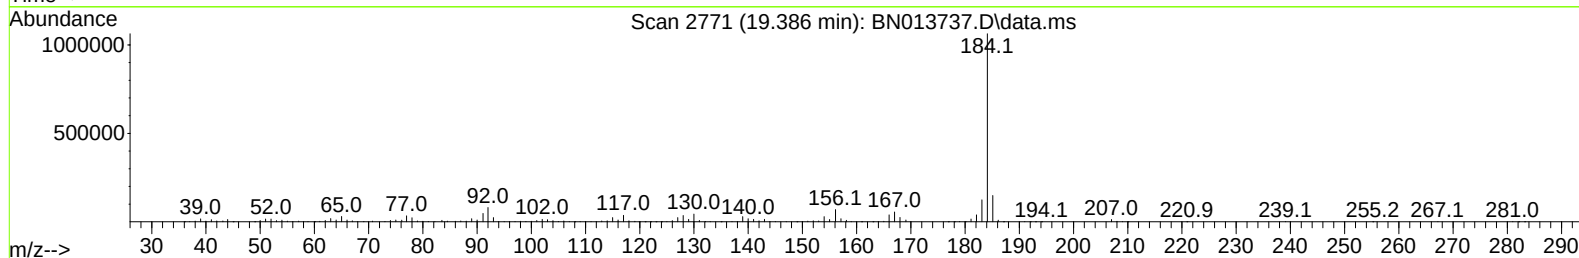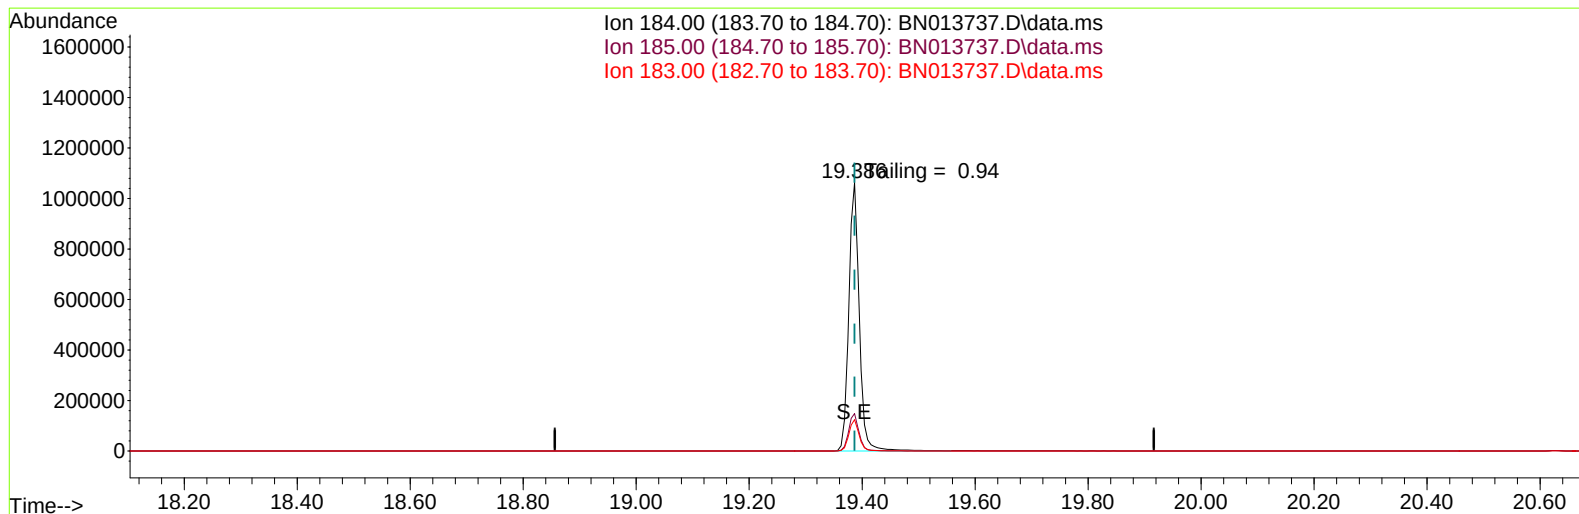

TIC: BN013737.D\data.ms

(77) Benzidine

19.386min (0.000) 0.00 ng

response 1374558

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.96
183.00	13.20	11.71
0.00	0.00	0.00