
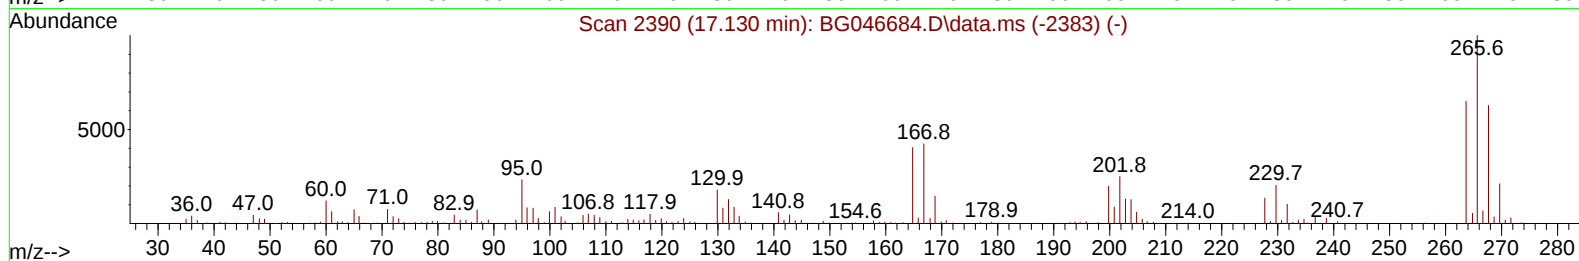
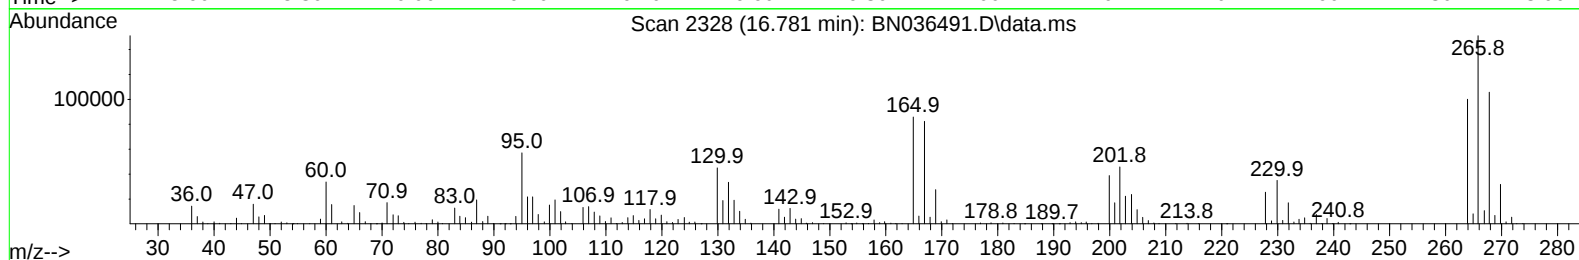


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022425\
Data File : BN036491.D
Acq On : 24 Feb 2025 10:10
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 24 12:45:49 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

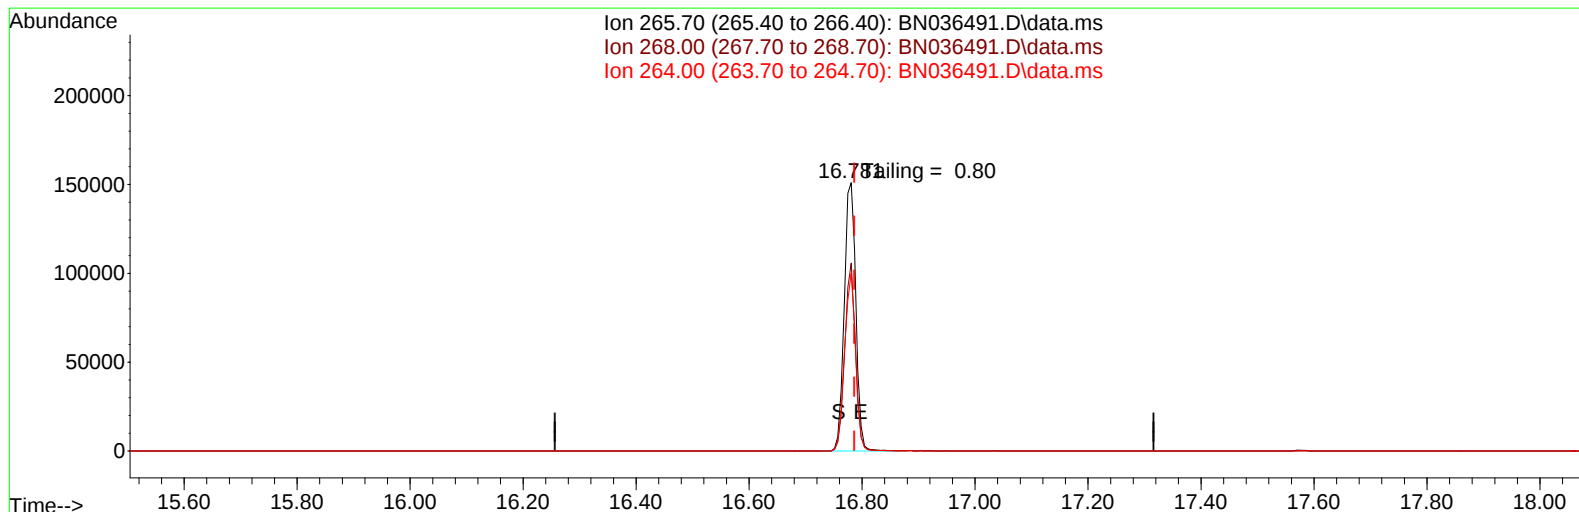

TIC: BN036491.D\data.ms

(70) Pentachlorophenol (C)




16.781min (-0.005) 19002.28 ng

response 213398

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	69.99
264.00	61.60	66.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022425\
Data File : BN036491.D
Acq On : 24 Feb 2025 10:10
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 24 12:45:49 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

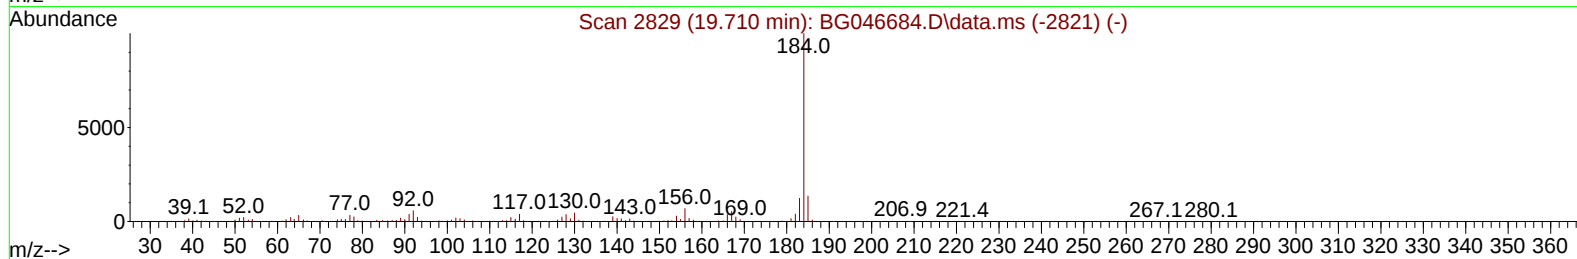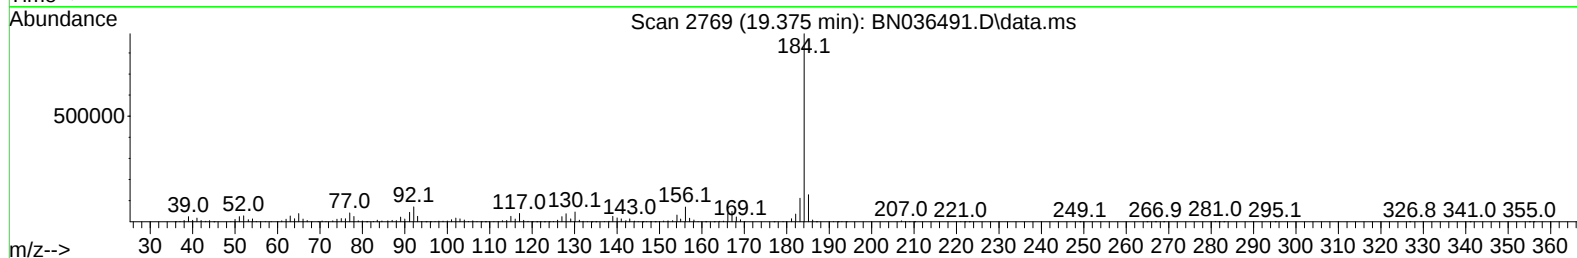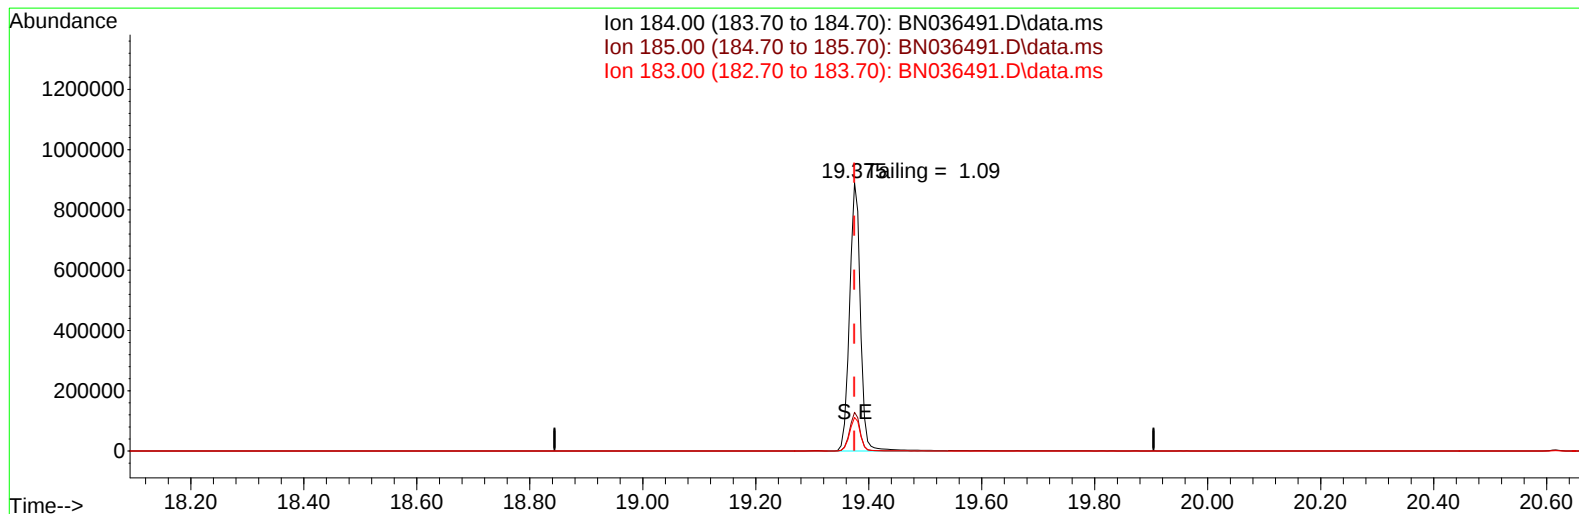

TIC: BN036491.D\data.ms

(77) Benzidine

19.375min (+ 0.001) 0.00 ng

response 1188729

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.43
183.00	13.20	12.54
0.00	0.00	0.00