

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN022519\
 Data File : BN004477.D
 Acq On : 25 Feb 2019 10:49
 Operator : JU/SJ
 Sample : PB117306BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK06

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020719MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.246	41	44	50	rVB3	2521	3697	0.29%	0.048%
2	6.899	660	665	672	rBB	69564	104440	8.15%	1.363%
3	7.081	691	696	708	rBB	52113	79648	6.22%	1.039%
4	7.269	723	728	735	rBB	75636	114450	8.93%	1.493%
5	7.740	803	808	814	rBB	66709	101731	7.94%	1.327%
6	8.434	920	926	933	rBB	98371	146204	11.41%	1.908%
7	8.905	1000	1006	1012	rBB	68540	110296	8.61%	1.439%
8	9.616	1121	1127	1133	rBB	55596	83978	6.55%	1.096%
9	10.140	1210	1216	1223	rBB	104485	162351	12.67%	2.118%
10	10.528	1275	1282	1289	rBB	115186	183435	14.32%	2.393%
11	10.669	1300	1306	1316	rBB	121285	192586	15.03%	2.513%
12	12.116	1549	1552	1555	rBB	1225	1345	0.10%	0.018%
13	13.793	1831	1837	1843	rBB	220483	300534	23.45%	3.921%
14	14.075	1879	1885	1892	rBV	270925	379614	29.63%	4.953%
15	14.381	1931	1937	1943	rBB2	198548	291678	22.76%	3.806%
16	14.575	1965	1970	1976	rBB	87810	119992	9.36%	1.566%
17	15.375	2100	2106	2112	rVB	377611	515480	40.23%	6.726%
18	15.493	2121	2126	2131	rBV	79296	98747	7.71%	1.288%
19	15.616	2144	2147	2151	rVB	1778	2208	0.17%	0.029%
20	17.128	2397	2404	2411	rBV2	284059	395261	30.85%	5.157%
21	17.228	2415	2421	2429	rBV	428841	589244	45.99%	7.688%
22	19.163	2746	2750	2754	rBV	3414	4009	0.31%	0.052%
23	19.416	2790	2793	2797	rBV	2460	2860	0.22%	0.037%
24	19.534	2807	2813	2823	rVB	596325	797553	62.24%	10.407%
25	21.328	3113	3118	3124	rBV	546668	671930	52.44%	8.767%
26	21.904	3214	3216	3221	rVB4	4829	5976	0.47%	0.078%
27	22.375	3293	3296	3299	rBV	6703	7711	0.60%	0.101%
28	22.886	3380	3383	3388	rVB2	11437	13649	1.07%	0.178%
29	23.457	3472	3480	3491	rBV	692393	1281340	100.00%	16.719%
30	23.604	3497	3505	3514	rVB	459115	843575	65.84%	11.007%
31	24.110	3587	3591	3600	rVB	15313	29737	2.32%	0.388%
32	24.869	3716	3720	3728	rVB3	14389	28711	2.24%	0.375%

LSC Area Percent Report

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN022519\
Data File : BN004477.D
Acq On : 25 Feb 2019 10:49
Operator : JU/SJ
Sample : PB117306BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK06

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020719MA.M
Title : SVOA CALIBRATION


Sum of corrected areas: 7663970

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN022519\
Data File : BN004477.D
Acq On : 25 Feb 2019 10:49
Operator : JU/SJ
Sample : PB117306BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK06

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020719MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

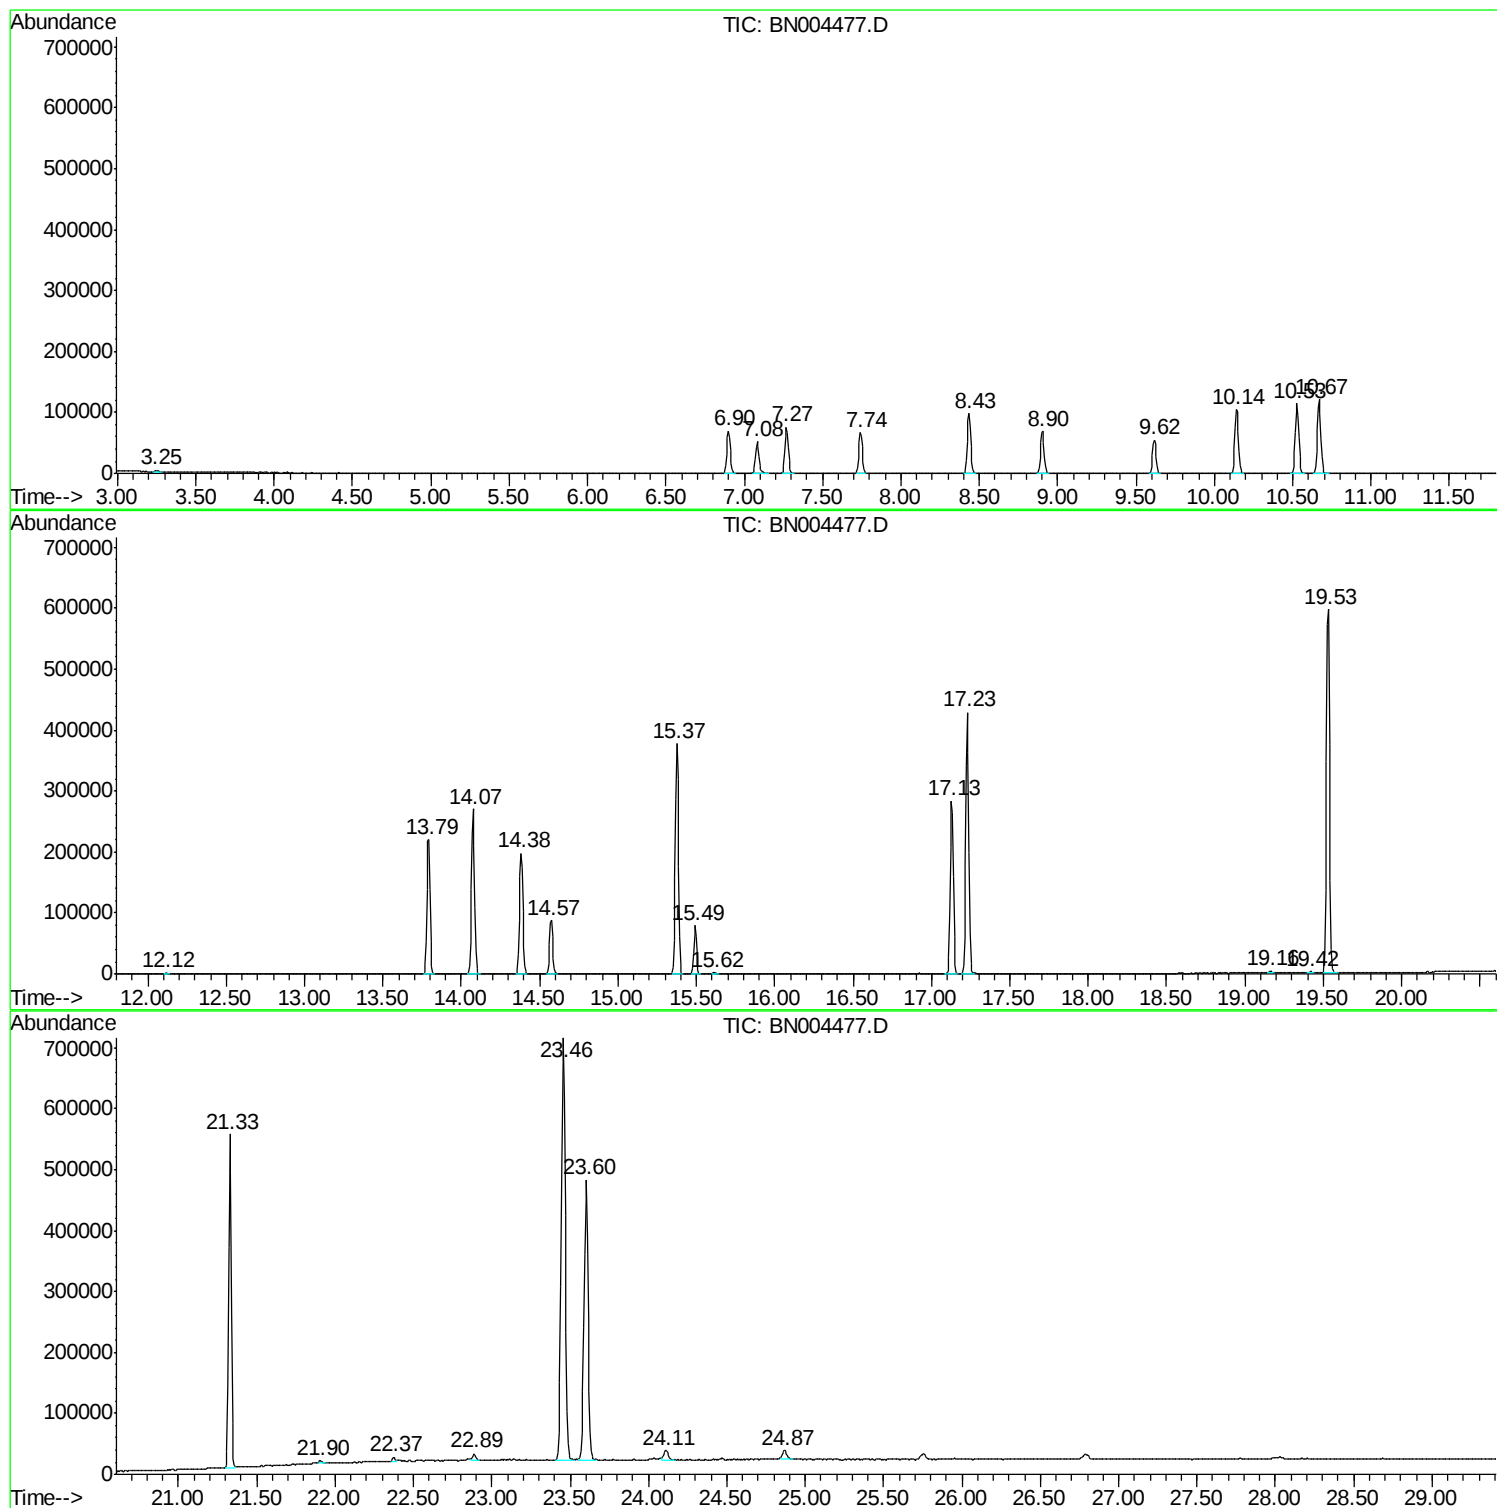

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN022519\
Data File : BN004477.D
Acq On : 25 Feb 2019 10:49
Operator : JU/SJ
Sample : PB117306BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK06

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020719MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN022519\
Data File : BN004477.D
Acq On : 25 Feb 2019 10:49
Operator : JU/SJ
Sample : PB117306BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK06

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020719MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc