


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022519\
 Data File : BN004475.D
 Acq On : 25 Feb 2019 09:38
 Operator : JU/SJ
 Sample : DFTPP08
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP08

Integration File: LSCINT.P

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN020719MA.M
 Title : SVOA CALIBRATION
 Last Update : Mon Feb 25 23:23:32 2019

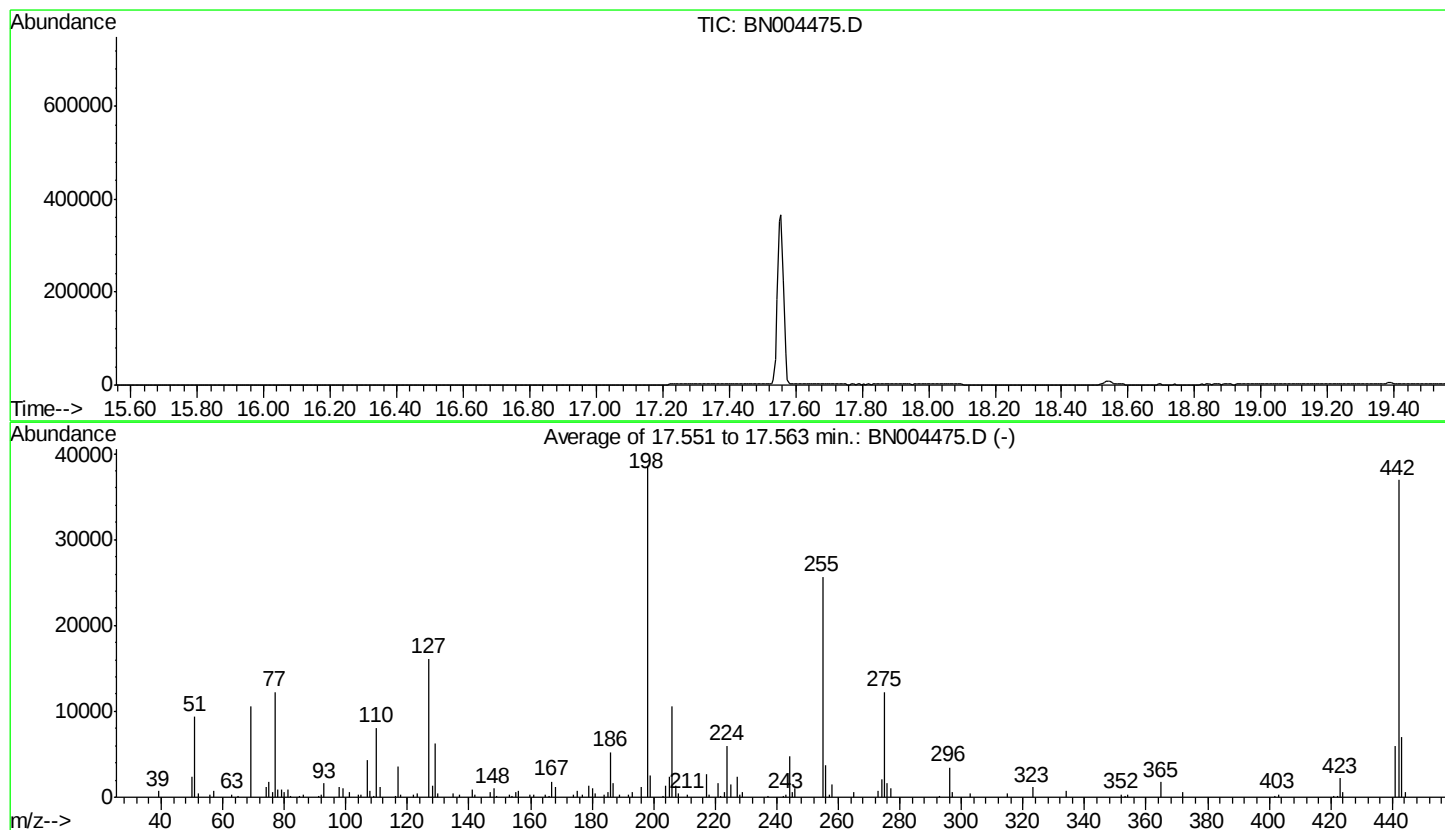

AutoFind: Scans 2476, 2477, 2478; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.2	9351	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	27.3	10542	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.8	16130	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	38600	PASS
199	198	5	9	6.7	2592	PASS
275	198	10	60	31.8	12294	PASS
365	198	1	100	4.5	1727	PASS
441	198	0.01	100	15.5	5998	PASS
442	198	50	100	95.7	36928	PASS
443	442	15	24	19.0	7014	PASS

Scan 2471 (17.522 min): BN004475.D
DFTPP08

m/z	Abundance
43.90	545.0
185.00	436.0
186.00	519.0
207.00	449.0

Instrument :
BNA_N
ClientSampleId :
DFTPP08

m/z	Abundance
39.00	912.0
44.00	539.0
50.00	3015.0
51.00	11669.0
52.00	649.0
55.90	392.0
57.00	850.0
63.00	493.0
65.00	376.0
69.00	12820.0
74.00	1493.0
75.00	2264.0
76.10	705.0
77.00	15211.0
78.00	1121.0
79.00	1106.0
80.00	847.0
81.00	1214.0
81.90	321.0
85.00	319.0
86.00	345.0
90.90	326.0
92.00	355.0
93.00	1937.0
98.00	1584.0
99.00	1298.0
100.90	711.0
104.00	478.0
104.90	455.0
107.00	5112.0
108.00	878.0
110.00	9979.0
111.00	1498.0
116.00	347.0
117.00	4354.0
117.90	405.0
121.90	418.0
123.00	637.0
127.00	19312.0
128.00	1591.0
129.00	7328.0
130.00	670.0
135.00	622.0
137.00	408.0
141.00	984.0
142.00	335.0
147.00	619.0
148.00	1205.0
149.00	314.0
152.90	393.0
154.00	328.0
155.00	671.0
156.00	851.0
159.90	367.0
161.00	457.0
165.00	410.0
166.00	335.0
167.00	2193.0
168.00	1470.0
174.00	447.0
175.00	879.0
177.00	454.0
178.90	1596.0
180.00	1177.0
180.90	578.0
183.90	331.0
185.00	1278.0
186.00	6791.0
187.00	1883.0
188.90	412.0
191.90	537.0
193.00	660.0
196.00	1334.0
198.00	44016.0
199.00	3120.0
203.00	342.0
204.00	1600.0
205.00	2771.0
206.00	12185.0
207.00	1968.0
208.00	462.0
210.90	491.0
217.00	3150.0
217.90	434.0
221.00	1901.0
223.00	691.0
224.00	6589.0
225.00	1659.0
227.00	2669.0
227.90	403.0
228.90	634.0

Instrument :
BNA_N
ClientSampleId :
DFTPP08

237.00	323.0
242.00	344.0
243.10	347.0
244.00	5381.0
245.00	718.0
245.90	1059.0
255.00	27792.0
256.00	4116.0
257.00	407.0
257.90	1636.0
265.00	652.0
273.00	787.0
274.00	2189.0
275.00	13023.0
276.00	1749.0
277.00	1021.0
296.00	3512.0
297.00	578.0
303.00	424.0
315.00	363.0
323.10	1324.0
334.00	768.0
352.00	331.0
353.00	318.0
354.10	367.0
365.00	1706.0
372.00	614.0
403.00	355.0
420.90	318.0
423.00	1973.0
424.00	590.0
441.10	5701.0
442.00	32640.0
443.00	6439.0
444.00	600.0

Instrument :
BNA_N
ClientSampleId :
DFTPP08

m/z	Abundance
39.00	775.0
44.00	483.0
50.00	2583.0
51.00	10690.0
52.00	624.0
55.90	319.0
57.00	788.0
63.00	508.0
69.00	12322.0
74.00	1244.0
75.00	2045.0
76.00	739.0
77.00	14096.0
78.00	977.0
79.00	1083.0
80.00	762.0
81.00	1070.0
82.00	307.0
86.00	372.0
91.00	351.0
91.90	343.0
93.00	1728.0
98.00	1397.0
99.00	1206.0
101.00	582.0
104.00	373.0
104.90	425.0
107.00	4928.0
107.90	752.0
109.00	328.0
110.00	9321.0
111.00	1355.0
116.10	307.0
117.00	3993.0
118.00	326.0
121.90	340.0
123.00	517.0
127.00	18680.0
128.00	1431.0
129.00	7181.0
130.00	572.0
135.00	616.0
137.00	373.0
141.00	1040.0
142.00	373.0
147.00	593.0
148.00	1052.0
153.00	366.0
154.00	343.0
155.00	614.0
156.00	768.0
159.90	328.0
161.00	435.0
164.90	349.0
166.10	353.0
167.00	1973.0
168.00	1318.0
174.00	491.0
175.00	807.0
176.90	402.0
179.00	1650.0
180.00	1161.0
181.00	486.0
184.00	373.0
185.00	1142.0
186.00	6522.0
187.00	1931.0
189.00	441.0
192.00	531.0
193.00	608.0
196.00	1251.0
198.00	44392.0
199.00	2921.0
203.00	325.0
204.00	1618.0
205.10	2785.0
206.00	12083.0
207.00	1994.0
208.00	533.0
211.00	494.0
217.00	3107.0
217.90	356.0
221.00	1898.0
221.80	467.0
223.00	710.0
224.00	6872.0
225.00	1730.0
227.00	2949.0
227.90	403.0
229.00	649.0
243.00	396.0

Instrument :
BNA_N
ClientSampleId :
DFTPP08

244.00	5683.0
245.00	728.0
246.00	1058.0
255.00	29600.0
256.00	4541.0
257.00	324.0
258.00	1801.0
265.00	681.0
273.00	982.0
274.00	2504.0
275.00	14282.0
276.00	1952.0
276.90	1121.0
293.00	329.0
296.00	4162.0
296.90	591.0
303.00	430.0
315.00	461.0
323.00	1306.0
334.00	905.0
352.00	461.0
354.00	457.0
365.00	2035.0
371.90	756.0
402.00	324.0
403.00	439.0
420.90	355.0
422.10	394.0
423.00	2560.0
424.00	655.0
441.10	7052.0
442.10	44048.0
443.00	8196.0
444.10	776.0

Instrument :
BNA_N
ClientSampleId :
DFTPP08

m/z	Abundance
39.00	412.0
43.90	548.0
50.00	1513.0
51.00	5694.0
57.00	538.0
69.00	6485.0
74.00	681.0
75.00	1161.0
76.00	350.0
77.00	7571.0
78.00	573.0
79.00	623.0
79.90	337.0
81.00	574.0
92.90	1068.0
98.00	761.0
99.00	637.0
101.00	383.0
107.00	2973.0
108.00	517.0
110.00	5020.0
111.00	830.0
117.00	2481.0
123.00	325.0
127.00	10398.0
128.00	818.0
129.00	4075.0
129.90	329.0
134.90	342.0
141.00	596.0
146.90	421.0
147.90	680.0
155.00	393.0
156.00	523.0
164.90	301.0
167.00	1231.0
168.00	633.0
174.90	544.0
178.90	897.0
180.00	651.0
180.90	309.0
185.00	901.0
186.00	4033.0
187.00	1237.0
193.00	451.0
196.00	866.0
198.00	27392.0
199.00	1736.0
204.00	1025.0
205.00	1764.0
206.00	7299.0
207.00	1466.0
208.00	339.0
217.00	1976.0
221.00	1308.0
223.00	489.0
224.00	4459.0
225.00	1197.0
227.00	1697.0
228.90	402.0
243.00	322.0
244.00	3415.0
245.10	503.0
246.00	812.0
255.00	19736.0
256.00	2747.0
258.00	1116.0
264.90	423.0
273.00	604.0
274.00	1583.0
275.00	9579.0
276.00	1244.0
277.00	849.0
296.00	2679.0
296.90	457.0
302.90	320.0
314.90	310.0
323.00	938.0
334.00	666.0
352.00	335.0
365.00	1440.0
372.00	588.0
403.00	307.0
423.10	2055.0
424.00	517.0
441.10	5241.0
442.10	34096.0
443.00	6409.0
444.00	517.0

Instrument :
BNA_N
ClientSampleId :
DFTPP08