

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022522\
 Data File : BN018735.D
 Acq On : 25 Feb 2022 17:42
 Operator : CG/JU
 Sample : N1656-06
 Misc :
 ALS Vial : 14 Sample Multiplier: 1




Instrument :
 BNA_N
 ClientSampleId :
 BGQ13

Manual IntegrationsAPPROVED

Quant Time: Feb 25 22:37:56 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN021622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Feb 16 16:48:14 2022
 Response via : Initial Calibration

Reviewed By :Jagrut
 Upadhyay

02/28/2022
 Supervised By :mohammad
 ahmed

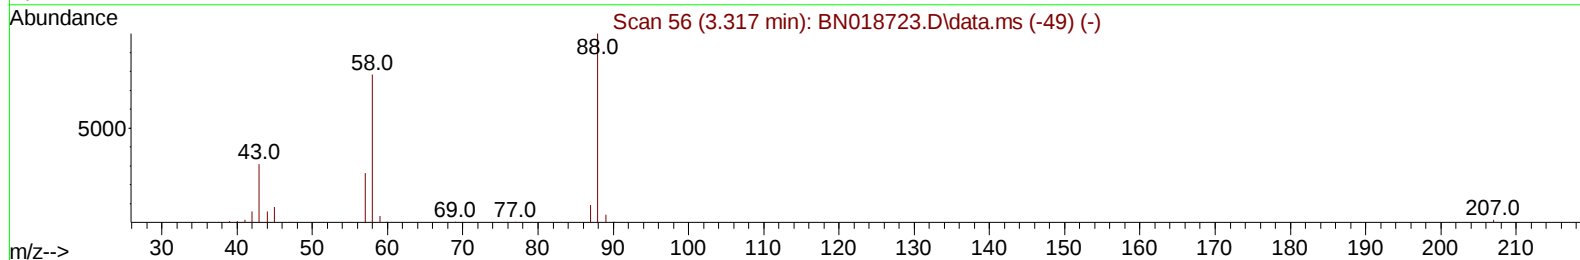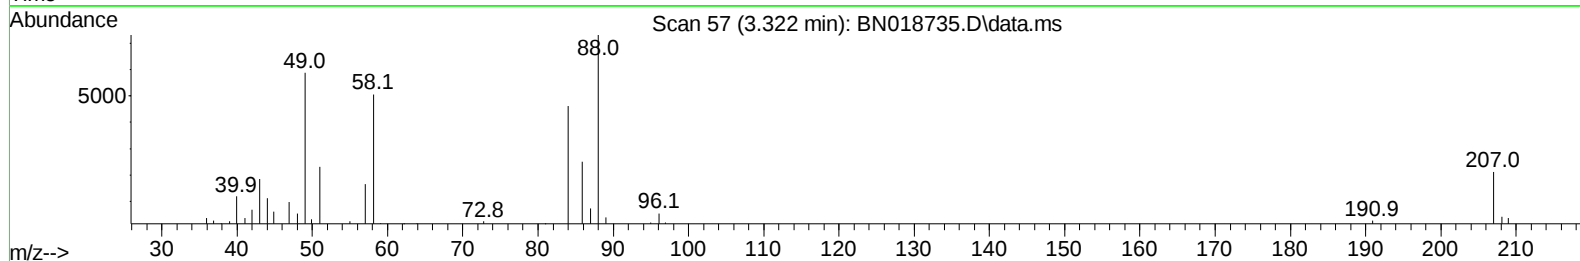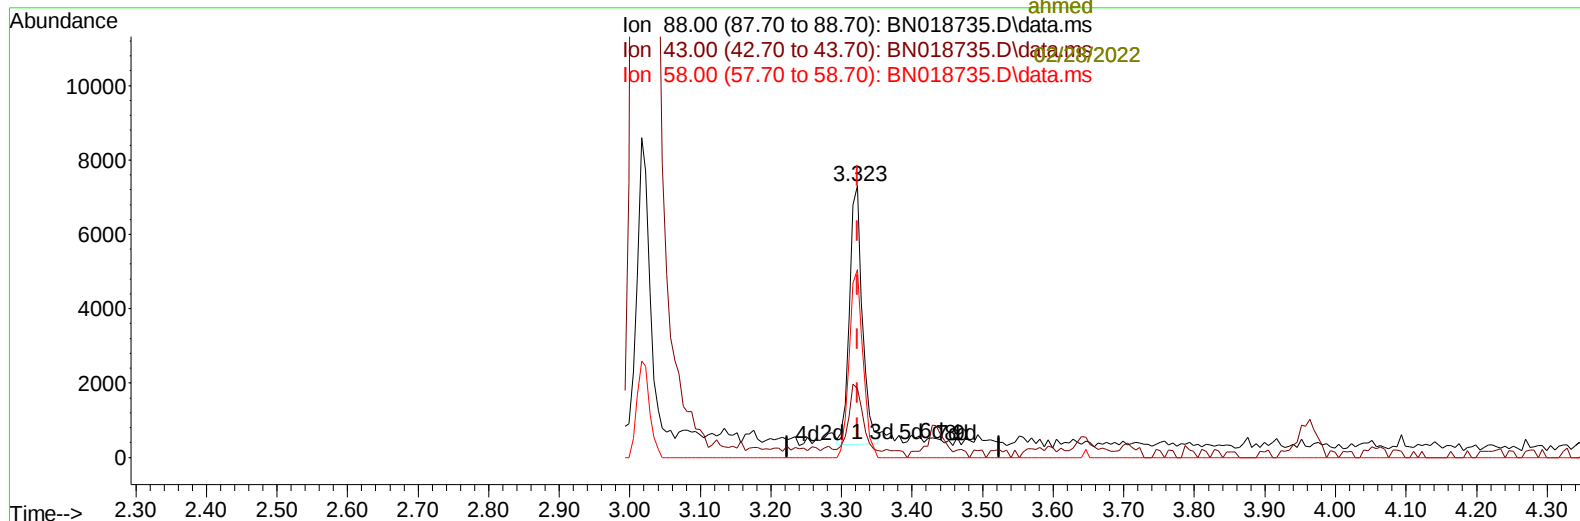

TIC: BN018735.D\data.ms

(2) 1,4-Dioxane

3.322min (-0.001) 1.76 ng/uL

response 8887

Ion	Exp%	Act%
88.00	100.00	100.00
43.00	27.40	25.27
58.00	70.40	69.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022522\
 Data File : BN018735.D
 Acq On : 25 Feb 2022 17:42
 Operator : CG/JU
 Sample : N1656-06
 Misc :
 ALS Vial : 14 Sample Multiplier: 1




Instrument :
 BNA_N
 ClientSampleId :
 BGQ13

Manual IntegrationsAPPROVED

Quant Time: Feb 25 22:37:56 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN021622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Feb 16 16:48:14 2022
 Response via : Initial Calibration

Reviewed By :Jagrut
 Upadhyay

02/28/2022
 Supervised By :mohammad
 ahmed

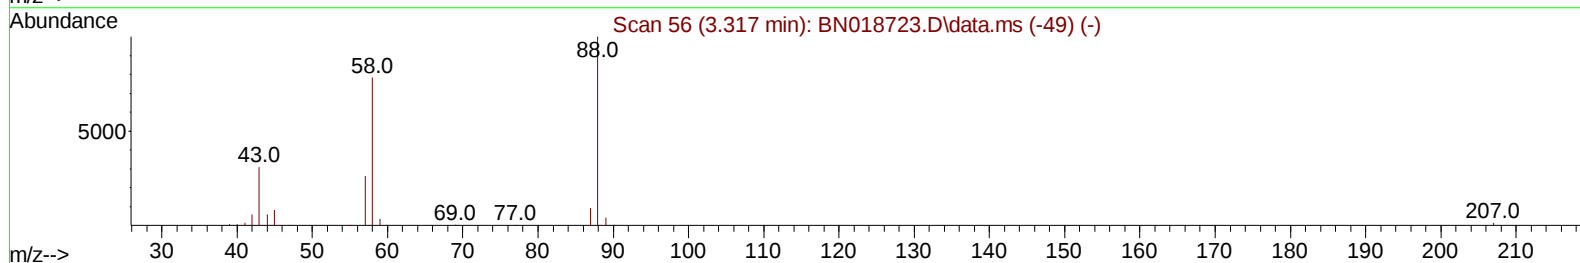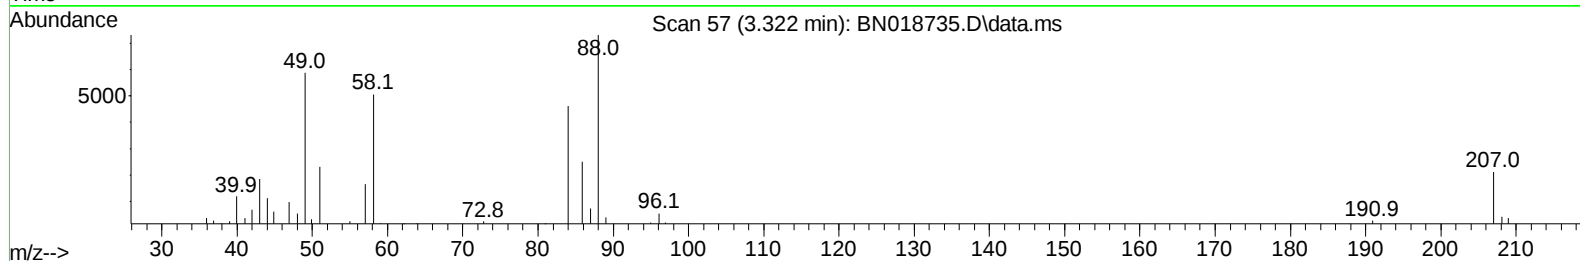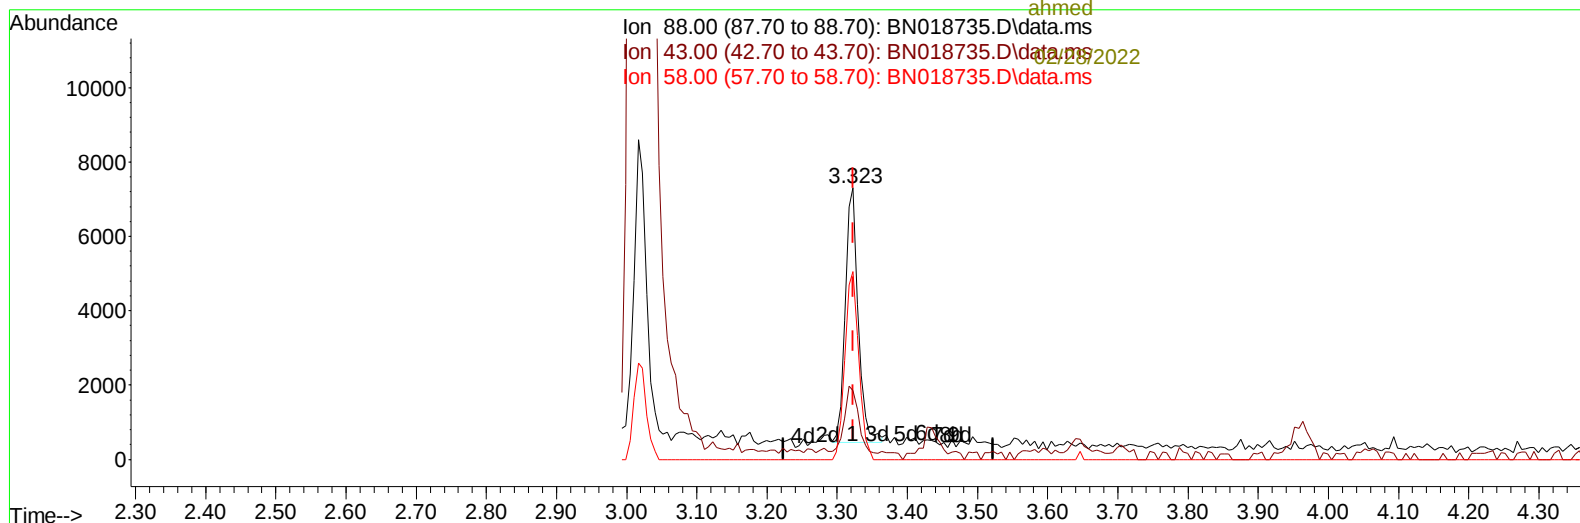

TIC: BN018735.D\data.ms

(2) 1,4-Dioxane

3.322min (-0.001) 1.71 ng/uL m

response 8650

Ion	Exp%	Act%
88.00	100.00	100.00
43.00	27.40	25.27
58.00	70.40	69.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022522\
 Data File : BN018735.D
 Acq On : 25 Feb 2022 17:42
 Operator : CG/JU
 Sample : N1656-06
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGQ13

Manual IntegrationsAPPROVED

Reviewed By :Jagrut
 Upadhyay

02/28/2022
 Supervised By :mohammad
 ahmed

Quant Time: Feb 25 22:37:56 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN021622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Feb 16 16:48:14 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)
-----02/28/2022							
Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.910	152		180466	20.000	ng/ul	0.00
20) Naphthalene-d8	10.716	136		682571	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.545	164		394214	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.286	188		788227	20.000	ng/ul	0.00
79) Chrysene-d12	21.463	240		814714	20.000	ng/ul	0.00
88) Perylene-d12	23.863	264		841761	20.000	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.281	96		20611	4.305	ng/uL	0.00
4) Pyridine-d5	3.705	84		77223	5.966	ng/ul	0.00
7) Phenol-d5	7.063	99		101361	6.810	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.234	67		291978	31.607	ng/ul	0.00
11) 2-Chlorophenol-d4	7.440	132		291905	24.901	ng/ul	0.00
15) 4-Methylphenol-d8	8.610	113		178737	15.725	ng/ul	0.00
21) Nitrobenzene-d5	9.069	128		164546	31.372	ng/ul	0.00
24) 2-Nitrophenol-d4	9.793	143		169503	30.175	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.334	165		296162	27.623	ng/ul	0.00
31) 4-Chloroaniline-d4	10.846	131		413899	28.893	ng/ul	0.00
46) Dimethylphthalate-d6	13.951	166		943557	33.063	ng/ul	0.00
49) Acenaphthylene-d8	14.240	160		1202380	32.521	ng/ul	0.00
54) 4-Nitrophenol-d4	14.722	143		23221	4.683	ng/ul	0.00
60) Fluorene-d10	15.534	176		856967	34.782	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.645	200		108533	23.337	ng/ul	0.00
73) Anthracene-d10	17.381	188		1389638	36.844	ng/ul	0.00
81) Pyrene-d10	19.675	212		1612641	33.818	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.710	264		1578015	36.759	ng/ul	0.00
Target Compounds							
2) 1,4-Dioxane	3.322	88		8650m	1.710	ng/uL	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN022522\
Data File : BN018735.D
Acq On : 25 Feb 2022 17:42
Operator : CG/JU
Sample : N1656-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGQ13

Manual IntegrationsAPPROVED

Reviewed By :Jagrut
Upadhyay

02/28/2022
Supervised By :mohammad
ahmed

Quant Time: Feb 25 22:37:56 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN021622.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 16 16:48:14 2022
Response via : Initial Calibration

